

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092920\
 Data File : VU040353.D
 Acq On : 29 Sep 2020 12:52
 Operator : SY/MD
 Sample : VU0929WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK16

Quant Time: Sep 30 02:00:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 30 01:43:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	137490	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	139224	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	63367	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	30847	4.53	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.60%
7) Chloroethane-d5	1.92	69	28606	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.00%
11) 1,1-Dichloroethene-d2	2.58	63	50209	3.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.40%
20) 2-Butanone-d5	4.65	46	167283	49.48	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.96%
24) Chloroform-d	5.08	84	72708	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
26) 1,2-Dichloroethane-d4	5.72	65	46173	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
32) Benzene-d6	5.74	84	132452	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
36) 1,2-Dichloropropane-d6	6.70	67	46983	4.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.80%
41) Toluene-d8	7.91	98	105814	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
43) trans-1,3-Dichloropropene-	8.19	79	19171	4.59	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.80%
46) 2-Hexanone-d5	8.64	63	118148	48.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.14%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	44781	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.00%
64) 1,2-Dichlorobenzene-d4	12.19	152	48025	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%


Target Compounds					Ovalue
16) Methylene chloride	3.06	84	2418	0.184 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092920\
Data File : VU040353.D
Acq On : 29 Sep 2020 12:52
Operator : SY/MD
Sample : VU0929WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK16

Quant Time: Sep 30 02:00:04 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Sep 30 01:43:05 2020
Response via : Initial Calibration

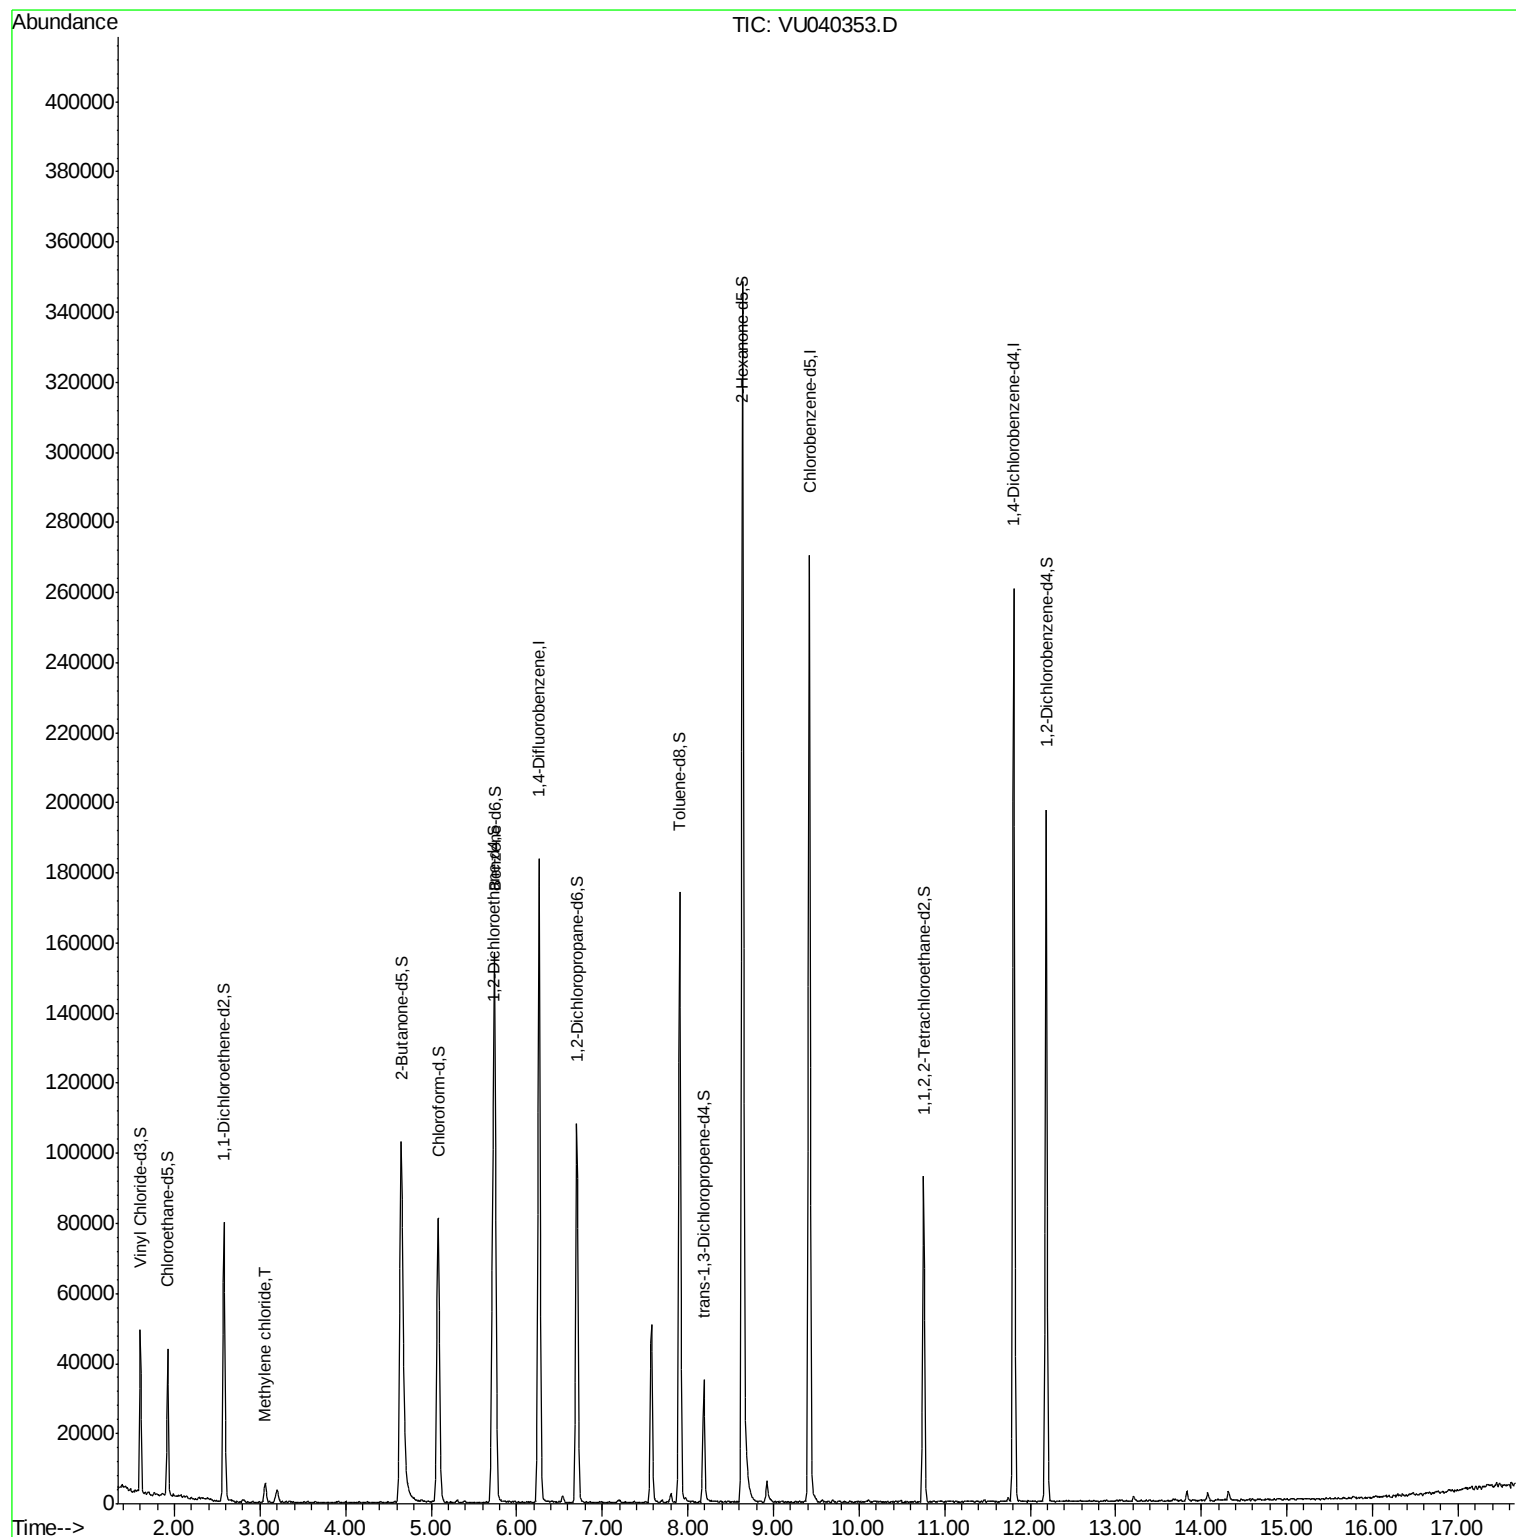

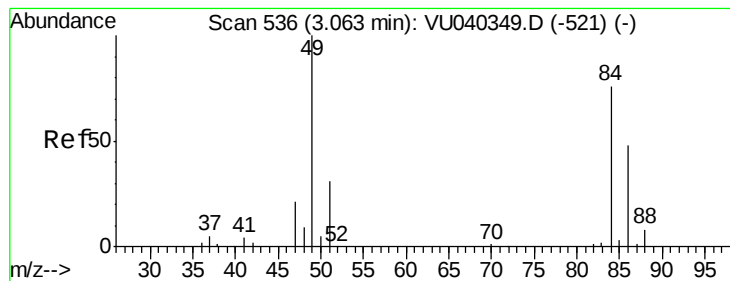

#16
Methylene chloride
Concen: 0.184 ug/L
RT: 3.06 min Scan# 536
Delta R.T. 0.00 min
Lab File: VU040353.D
Acq: 29 Sep 2020 12:52

Instrument :
MSVOA_U
ClientSampleId :
VBLK16

Tot Ion: 84 Resp: 2418

Ion	Ratio	Lower	Upper
84	100		
86	74.1	44.4	82.5
49	126.0	92.2	171.2

