

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092920\
 Data File : VU040363.D
 Acq On : 29 Sep 2020 16:51
 Operator : SY/MD
 Sample : L4164-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AE1

Quant Time: Sep 30 02:37:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 30 01:43:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	127861	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	129066	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	57037	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	28596	4.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.40%
7) Chloroethane-d5	1.92	69	27635	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.80%
11) 1,1-Dichloroethene-d2	2.58	63	47175	3.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.00%
20) 2-Butanone-d5	4.65	46	156963	49.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.84%
24) Chloroform-d	5.08	84	73550	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	5.72	65	45399	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
32) Benzene-d6	5.74	84	127796	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.70	67	46817	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	7.91	98	100880	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.60%
43) trans-1,3-Dichloropropene-	8.19	79	17674	4.56	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.20%
46) 2-Hexanone-d5	8.64	63	109323	47.98	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.96%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	43648	4.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	46093	5.33	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.60%


Target Compounds					Ovalue
13) Acetone	2.65	43	3156	1.205 ug/L	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092920\
Data File : VU040363.D
Acq On : 29 Sep 2020 16:51
Operator : SY/MD
Sample : L4164-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AE1

Quant Time: Sep 30 02:37:09 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Sep 30 01:43:05 2020
Response via : Initial Calibration

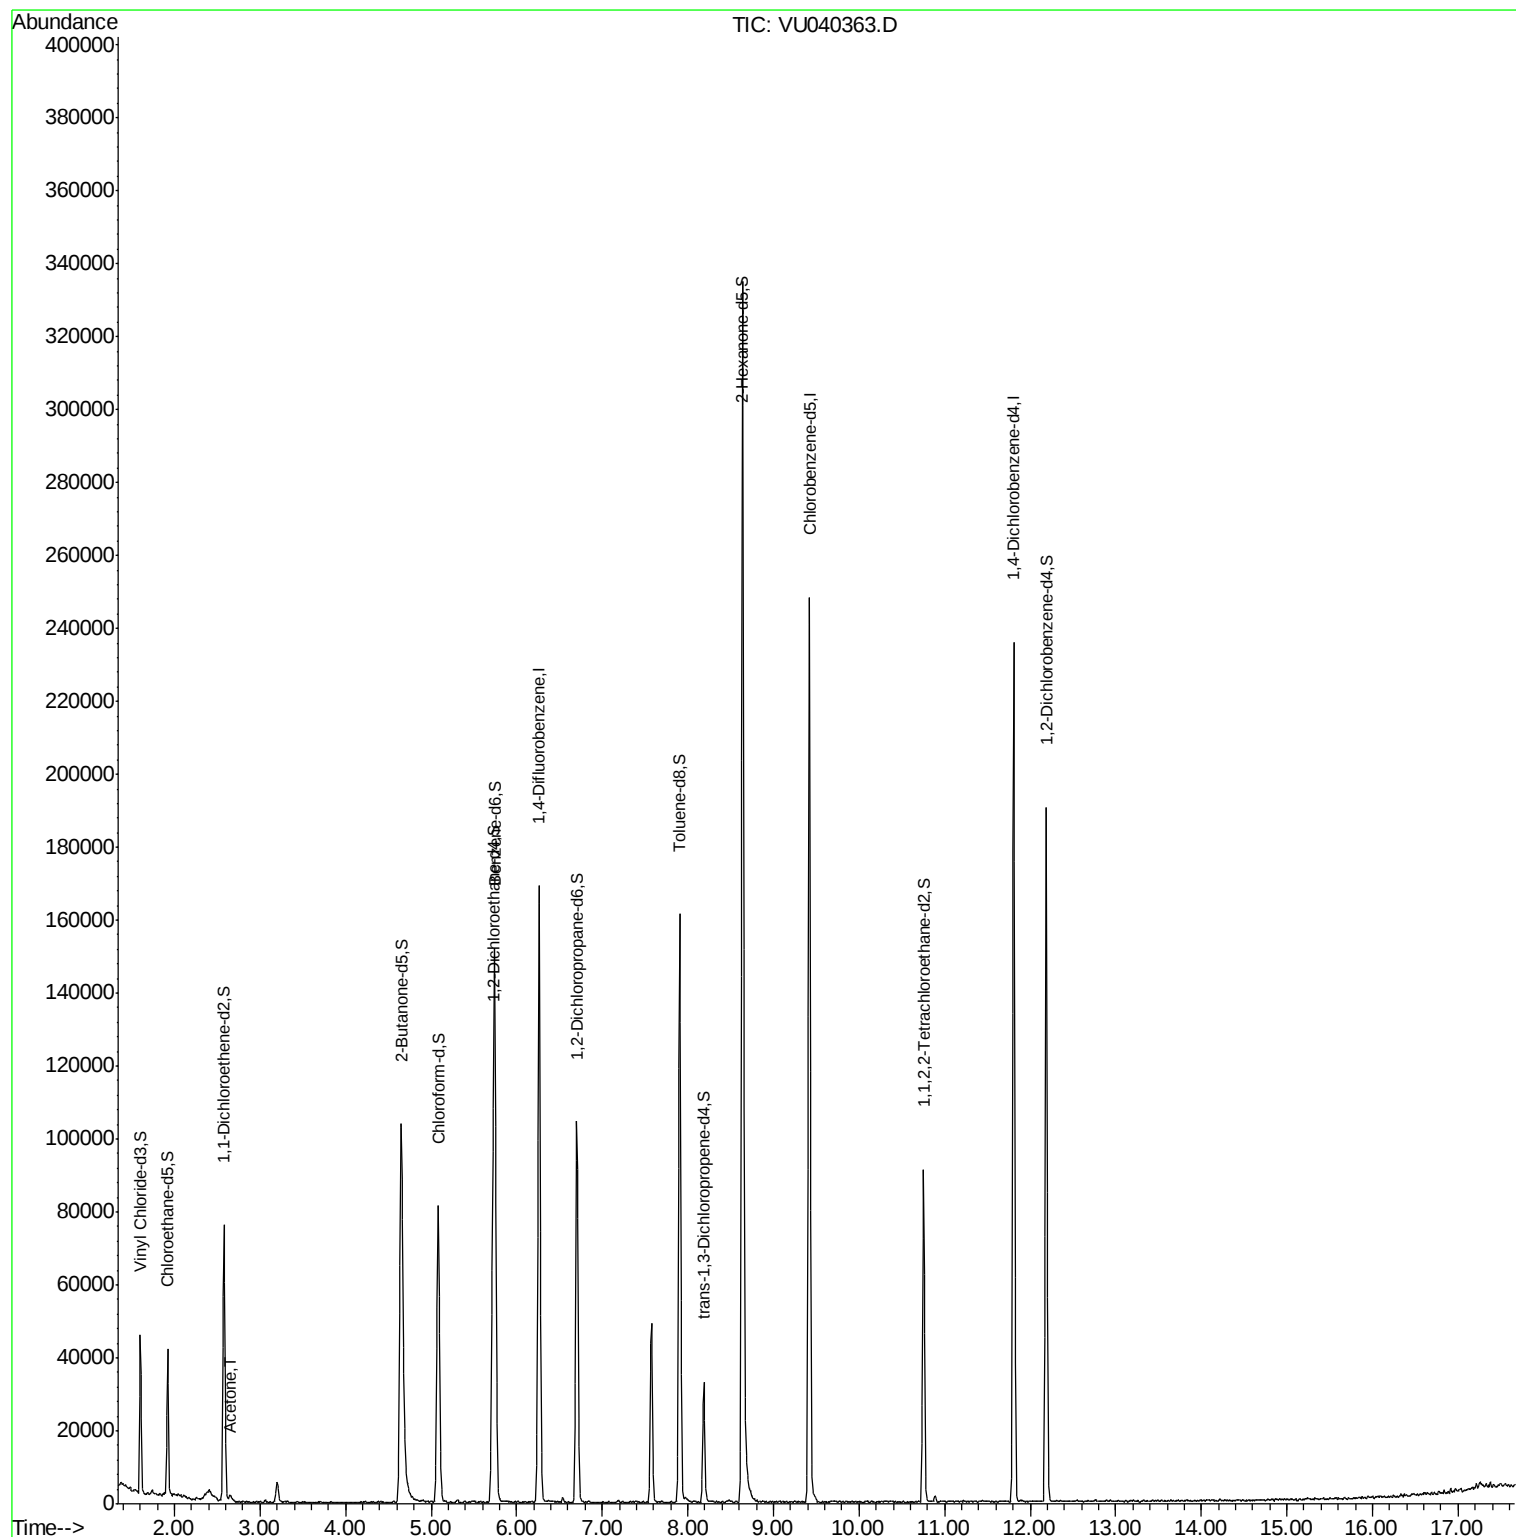

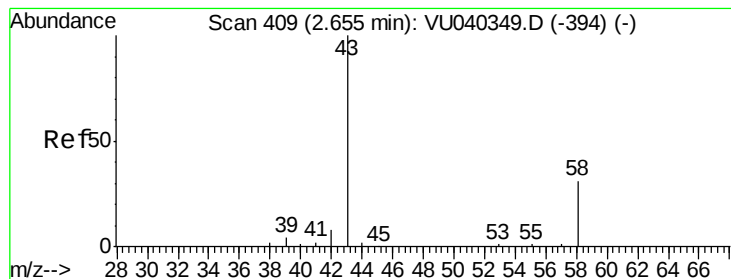

#13
 Acetone
 Concen: 1.205 ug/L
 RT: 2.65 min Scan# 408
 Delta R.T. -0.00 min
 Lab File: VU040363.D
 Acq: 29 Sep 2020 16:51

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AE1

Tot Ion: 43 Resp: 3156
 Ion Ratio Lower Upper
 43 100
 58 12.7 0.0 61.8

