

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092920\
 Data File : VU040364.D
 Acq On : 29 Sep 2020 17:14
 Operator : SY/MD
 Sample : L4164-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AE2

Quant Time: Sep 30 02:40:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 30 01:43:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	128734	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	132572	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	60256	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	29367	4.61	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.20%
7) Chloroethane-d5	1.92	69	29391	5.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.40%
11) 1,1-Dichloroethene-d2	2.58	63	49470	3.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.60%
20) 2-Butanone-d5	4.65	46	166920	52.73	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.46%
24) Chloroform-d	5.08	84	75052	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	5.72	65	48324	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.60%
32) Benzene-d6	5.75	84	132603	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	6.70	67	48831	5.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.20%
41) Toluene-d8	7.91	98	104040	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
43) trans-1,3-Dichloropropene-	8.19	79	18609	4.68	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.60%
46) 2-Hexanone-d5	8.64	63	121032	51.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.44%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	46173	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	48771	5.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.80%


Target Compounds					Ovalue
13) Acetone	2.66	43	3935	1.492 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092920\
Data File : VU040364.D
Acq On : 29 Sep 2020 17:14
Operator : SY/MD
Sample : L4164-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AE2

Quant Time: Sep 30 02:40:38 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Sep 30 01:43:05 2020
Response via : Initial Calibration

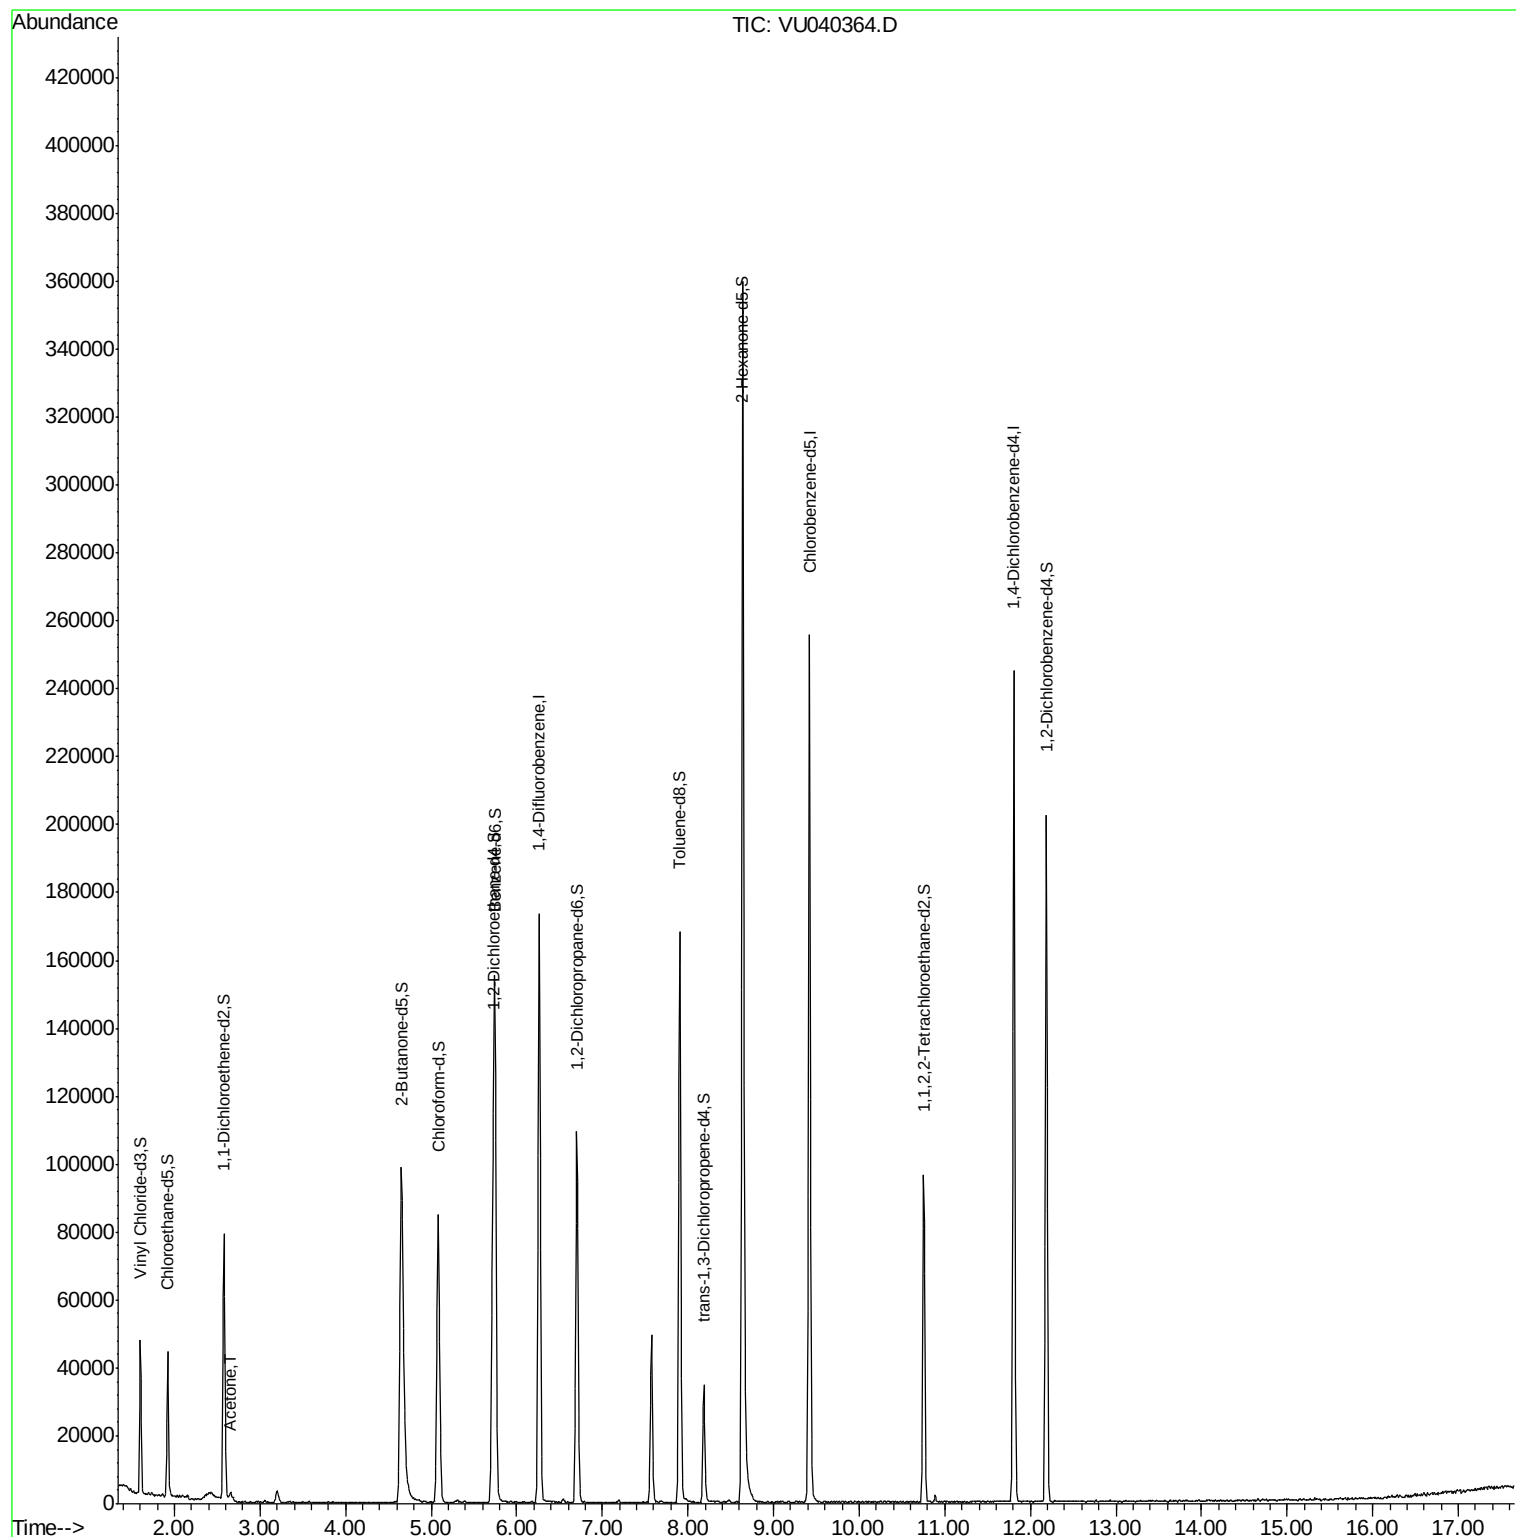

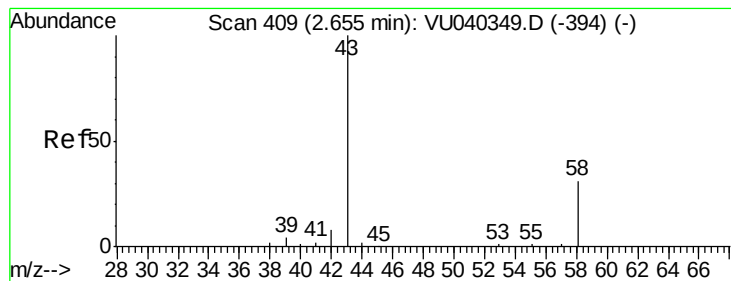

#13
 Acetone
 Concen: 1.492 ug/L
 RT: 2.66 min Scan# 410
 Delta R.T. 0.00 min
 Lab File: VU040364.D
 Acq: 29 Sep 2020 17:14

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AE2

Tot Ion: 43 Resp: 3935
 Ion Ratio Lower Upper
 43 100
 58 25.5 0.0 61.8

