


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092920\
 Data File : VU040346.D
 Acq On : 29 Sep 2020 08:53
 Operator : SY/MD
 Sample : BFB09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB09

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Sep 30 02:48:48 2020

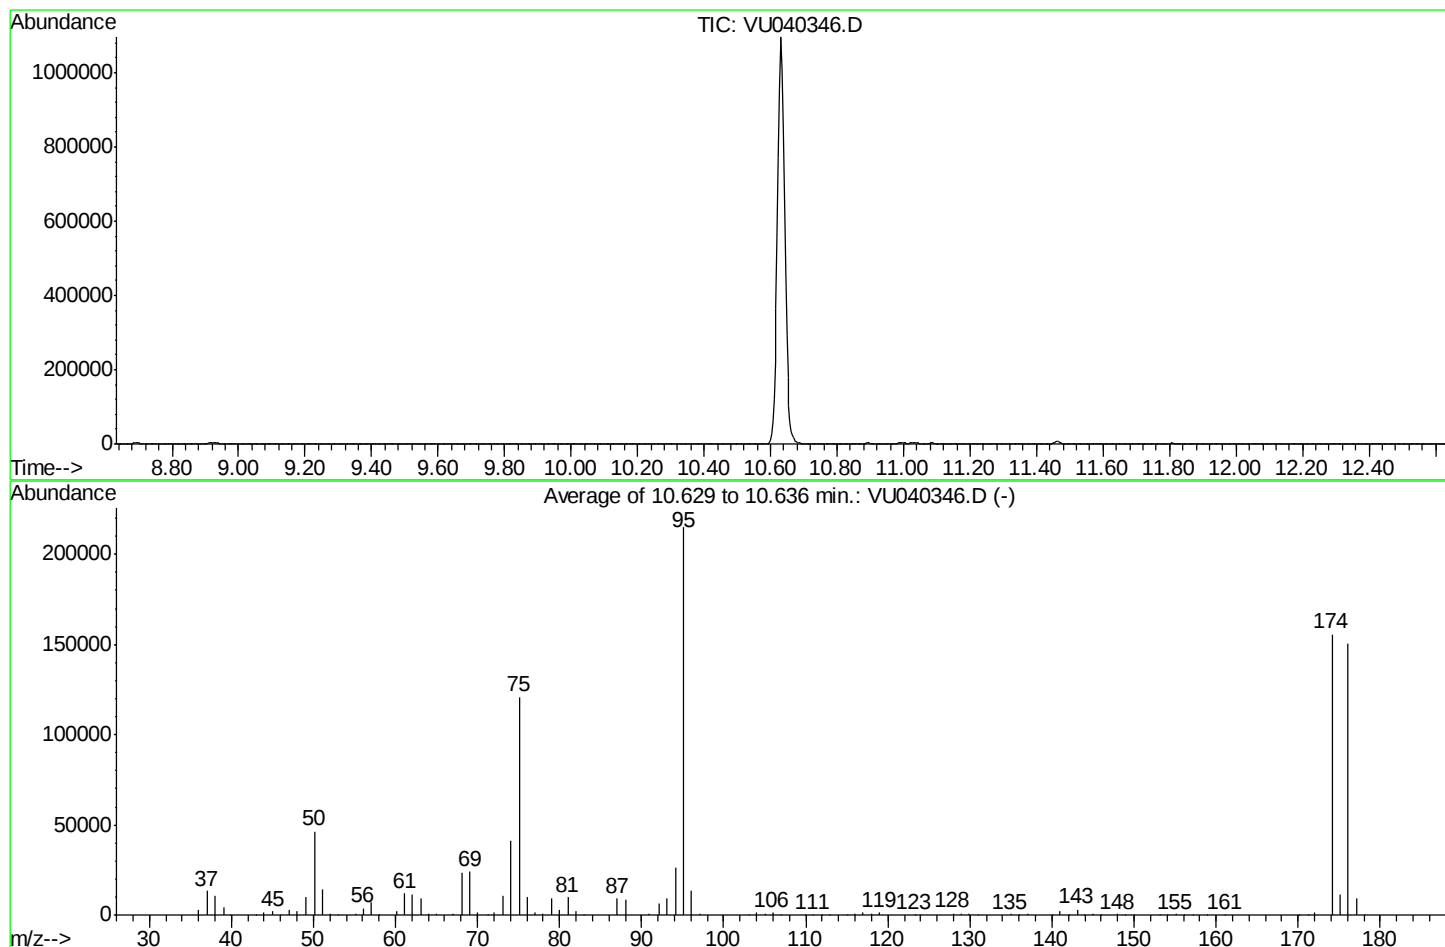

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	46290	PASS
75	95	30	80	56.2	120890	PASS
95	95	100	100	100.0	214976	PASS
96	95	5	9	6.4	13725	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.5	155776	PASS
175	174	5	9	7.4	11598	PASS
176	174	95	101	96.5	150336	PASS
177	176	5	9	6.2	9301	PASS

m/z	Abundance
36.00	2663.0
37.00	13802.0
38.00	11023.0
39.10	4475.0
40.00	316.0
43.00	115.0
44.00	2123.0
45.00	2119.0
46.00	396.0
47.10	2907.0
48.00	2058.0
49.10	10805.0
50.10	47864.0
51.10	14862.0
52.10	588.0
52.90	216.0
55.10	712.0
56.10	3574.0
57.10	7515.0
58.00	351.0
60.10	2240.0
61.10	12098.0
62.10	11850.0
63.10	9963.0
64.00	1139.0
65.10	1193.0
67.00	706.0
68.10	23848.0
69.10	24176.0
70.00	1772.0
72.00	1388.0
73.10	10853.0
74.10	43040.0
75.10	123328.0
76.10	10478.0
77.00	1307.0
78.00	913.0
79.00	9737.0
80.00	2664.0
81.00	9924.0
82.00	2468.0
83.00	179.0
87.00	9382.0
88.10	8693.0
90.90	1081.0
92.10	6355.0
93.10	9644.0
94.10	27144.0
95.10	219584.0
96.10	13953.0
97.00	402.0
103.00	121.0
104.00	1175.0
105.00	450.0
106.00	1298.0
107.00	234.0
109.80	150.0
110.90	225.0
111.90	180.0
112.90	202.0
115.00	326.0
116.00	923.0
117.00	1322.0
118.00	1038.0
119.00	1443.0
123.90	186.0
128.00	825.0
129.00	496.0
129.90	727.0
131.00	289.0
134.90	508.0
135.90	119.0
137.00	408.0
140.10	133.0
141.00	2458.0
142.10	352.0
143.00	3257.0
143.90	165.0
145.00	588.0
146.00	349.0
148.00	619.0
148.90	144.0
149.90	293.0
153.10	100.0
155.10	567.0
156.10	123.0
157.10	363.0
159.00	210.0
161.10	202.0
170.10	104.0
171.20	240.0
172.00	1873.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

174.10	155136.0
175.10	11646.0
176.10	148928.0
177.10	9089.0
178.00	258.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.00	2568.0
37.00	13723.0
38.00	10694.0
39.10	4439.0
40.00	294.0
43.10	133.0
44.00	2081.0
45.10	2116.0
46.00	365.0
47.10	3026.0
48.00	2043.0
49.10	10573.0
50.10	47728.0
51.10	14312.0
52.10	593.0
52.90	184.0
55.10	772.0
56.10	3750.0
57.10	7306.0
58.00	294.0
60.10	2277.0
61.10	12280.0
62.10	12050.0
63.10	9820.0
64.00	1104.0
65.10	1070.0
67.00	775.0
68.10	24168.0
69.10	24864.0
70.00	1740.0
72.10	1413.0
73.10	10928.0
74.10	42760.0
75.10	124784.0
76.10	10026.0
77.10	1279.0
78.00	892.0
79.00	9828.0
80.00	2745.0
81.00	10044.0
82.00	2424.0
83.00	229.0
87.00	9502.0
88.00	8390.0
90.90	1093.0
92.10	6392.0
93.10	9687.0
94.10	27360.0
95.10	222016.0
96.10	14167.0
97.10	442.0
103.00	135.0
104.00	1127.0
105.00	416.0
106.00	1328.0
107.00	259.0
109.90	206.0
110.90	257.0
111.90	196.0
112.90	150.0
115.00	322.0
116.00	933.0
117.00	1314.0
118.00	959.0
119.00	1335.0
123.90	216.0
128.00	851.0
129.00	477.0
129.90	763.0
131.00	299.0
135.00	529.0
135.90	126.0
137.00	405.0
140.00	174.0
141.00	2510.0
142.10	399.0
143.00	3167.0
143.90	171.0
145.00	590.0
146.00	394.0
148.00	572.0
148.90	133.0
149.90	310.0
153.10	139.0
154.00	129.0
155.10	667.0
156.10	110.0
157.10	384.0
158.90	225.0
161.10	202.0
170.10	132.0
171.10	265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

172.00	1598.0
174.10	160960.0
175.10	11933.0
176.10	155456.0
177.10	9523.0
178.10	257.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.00	2334.0
37.00	12150.0
38.00	9707.0
39.10	4132.0
39.90	309.0
43.10	119.0
44.00	1801.0
45.10	1961.0
46.00	295.0
47.10	2752.0
48.00	1703.0
49.10	9536.0
50.10	43280.0
51.10	12463.0
52.10	566.0
53.00	116.0
55.10	693.0
56.10	3529.0
57.10	6323.0
58.00	246.0
60.10	2131.0
61.10	11389.0
62.10	11072.0
63.10	8690.0
64.10	943.0
65.00	987.0
67.00	748.0
68.10	22032.0
69.10	22944.0
70.00	1676.0
71.20	109.0
72.10	1307.0
73.10	10375.0
74.10	38632.0
75.10	114560.0
76.10	8790.0
77.00	1232.0
78.00	840.0
79.00	8936.0
80.00	2617.0
81.00	9369.0
82.00	2166.0
83.00	254.0
87.00	8654.0
88.00	7609.0
90.90	943.0
92.10	5962.0
93.10	8910.0
94.10	25016.0
95.10	203328.0
96.10	13056.0
97.10	418.0
103.10	133.0
104.00	981.0
105.00	359.0
106.00	1170.0
107.00	269.0
109.80	199.0
110.90	256.0
112.00	174.0
112.90	139.0
115.00	295.0
116.00	885.0
117.00	1254.0
118.00	798.0
119.00	1147.0
123.30	100.0
123.90	208.0
128.00	798.0
129.00	396.0
129.90	726.0
131.00	289.0
135.00	506.0
135.90	117.0
137.00	444.0
140.00	182.0
141.00	2241.0
142.10	353.0
143.10	2846.0
143.90	149.0
145.00	471.0
146.00	404.0
148.00	482.0
149.00	109.0
150.00	246.0
153.10	122.0
154.10	149.0
155.10	595.0
157.10	352.0
158.90	218.0
161.10	222.0
170.10	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

171.10	236.0
172.00	1347.0
174.10	151232.0
175.10	11216.0
176.10	146624.0
177.10	9293.0
178.10	281.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

Scan 2875 (10.584 min): VU040346.D
BFB09

m/z	Abundance
39.90	112.0
44.00	363.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09