


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092921\
Data File : VU044984.D
Acq On : 29 Sep 2021 10:36
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
Title : SW846 8260
Last Update : Tue Sep 28 12:32:13 2021

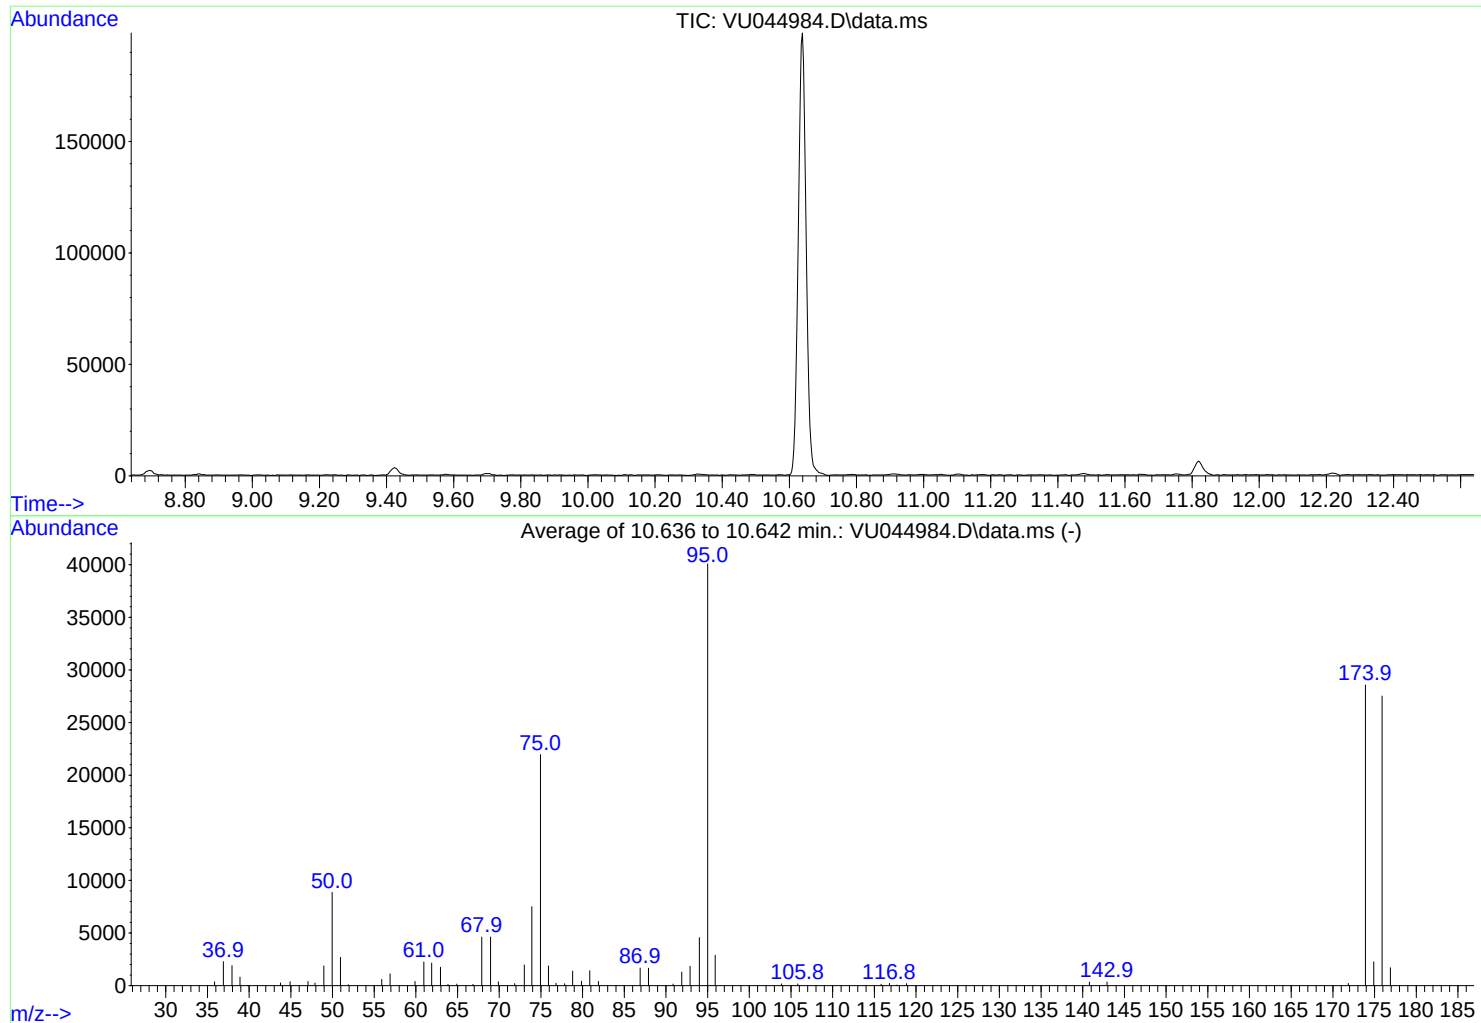

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.1	8860	PASS
75	95	30	60	54.8	21955	PASS
95	95	100	100	100.0	40083	PASS
96	95	5	9	7.2	2890	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.3	28571	PASS
175	174	5	9	7.9	2262	PASS
176	174	95	101	96.3	27525	PASS
177	176	5	9	6.2	1697	PASS