


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093019\
Data File : VU034875.D
Acq On : 30 Sep 2019 11:45
Operator : JC/SP
Sample : BFB12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB12

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR093019WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Sep 30 17:11:33 2019

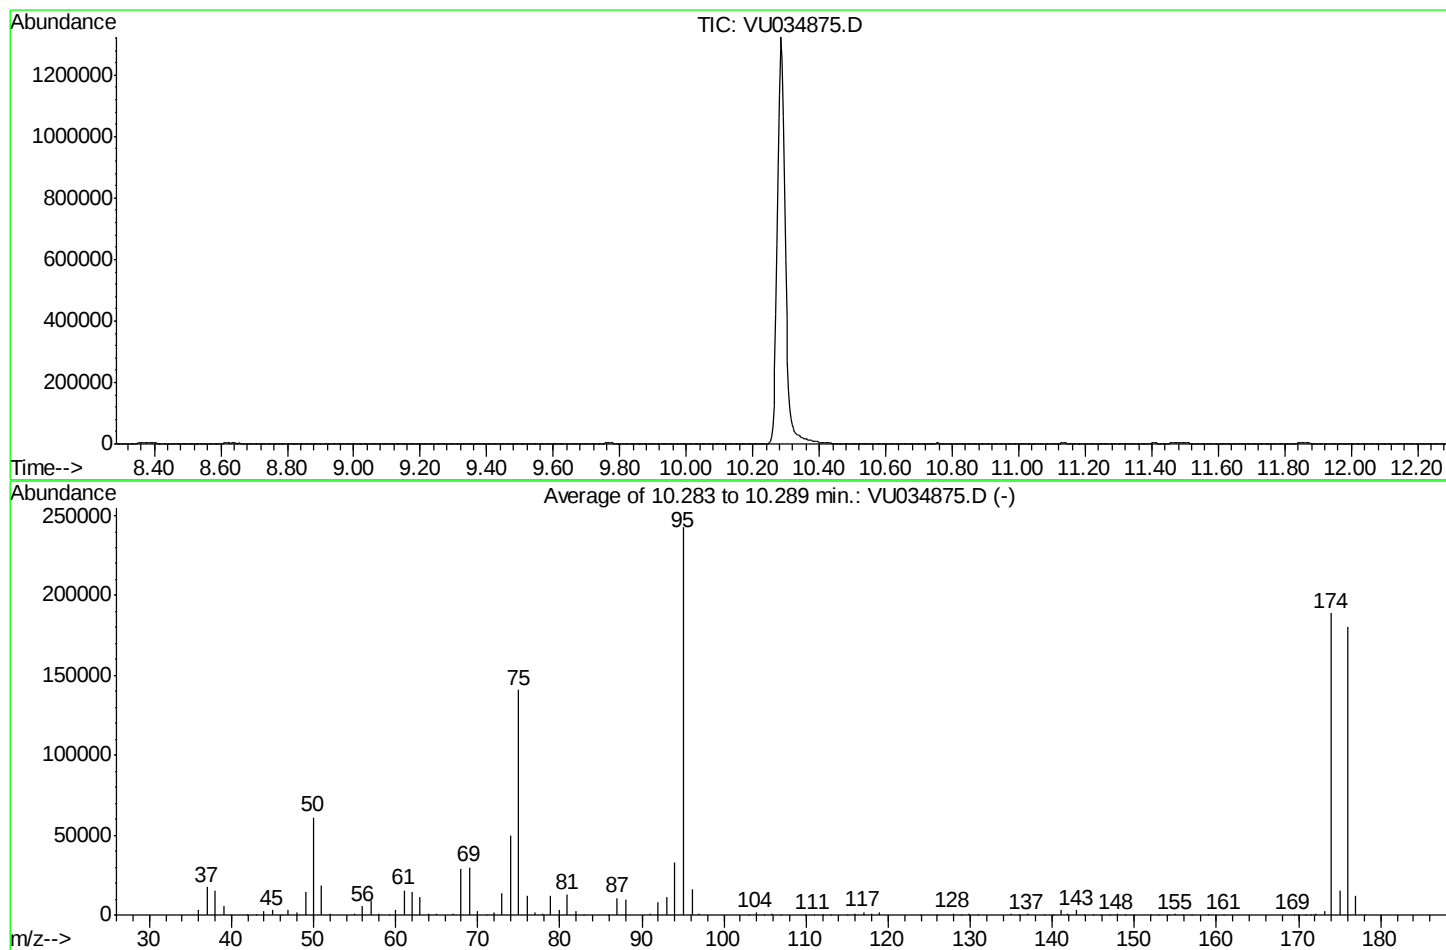

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.2	61248	PASS
75	95	30	80	58.1	140885	PASS
95	95	100	100	100.0	242688	PASS
96	95	5	9	6.6	16100	PASS
173	174	0.00	2	1.3	2465	PASS
174	95	50	120	77.8	188928	PASS
175	174	5	9	7.9	14929	PASS
176	174	95	101	95.6	180608	PASS
177	176	5	9	6.9	12415	PASS

m/z	Abundance
39.80	242.0
44.00	674.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	3319.0
37.00	18200.0
38.00	15530.0
39.00	5609.0
39.90	480.0
41.90	102.0
43.00	272.0
44.00	2899.0
45.00	3123.0
46.00	309.0
46.90	3473.0
48.00	1894.0
49.00	14116.0
50.00	62304.0
51.00	19472.0
52.00	987.0
55.00	932.0
56.00	5096.0
57.00	9015.0
58.00	452.0
60.00	3151.0
61.00	15654.0
62.00	15011.0
63.00	11840.0
64.10	1124.0
65.00	496.0
67.00	805.0
68.00	29336.0
69.00	30272.0
70.00	2428.0
71.00	121.0
72.00	1749.0
73.00	13718.0
74.00	50264.0
75.00	141312.0
76.10	12539.0
77.00	1663.0
77.90	1145.0
78.90	12340.0
79.90	3328.0
80.90	12558.0
81.90	2539.0
83.00	268.0
85.90	238.0
87.00	10553.0
88.00	9722.0
91.00	1200.0
92.00	8573.0
93.00	11542.0
94.00	33312.0
95.00	243584.0
96.10	16297.0
97.00	501.0
103.00	208.0
103.90	1456.0
105.00	438.0
105.90	1173.0
106.90	372.0
109.90	268.0
110.90	354.0
112.00	235.0
112.90	323.0
115.00	286.0
115.90	1244.0
117.00	1884.0
118.00	1100.0
119.00	1677.0
123.90	192.0
126.00	129.0
128.00	1069.0
129.00	477.0
129.90	980.0
131.00	372.0
134.90	475.0
137.00	632.0
140.10	250.0
141.00	2896.0
141.90	438.0
143.00	3258.0
143.90	239.0
145.00	325.0
146.00	333.0
147.00	220.0
147.90	545.0
148.90	191.0
149.90	298.0
152.90	108.0
154.20	123.0
155.00	417.0
155.80	111.0
157.00	431.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

158.90	265.0
160.90	311.0
169.40	210.0
169.90	170.0
170.80	259.0
172.00	1069.0
173.20	3689.0
174.00	184576.0
175.10	14924.0
176.00	176448.0
177.00	12471.0
178.00	312.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	3295.0
37.00	18064.0
38.00	15715.0
39.10	5413.0
39.90	511.0
43.00	263.0
44.00	2948.0
45.00	3126.0
46.00	297.0
47.00	3655.0
48.00	1873.0
49.00	14746.0
50.00	63120.0
51.00	19160.0
52.00	962.0
55.00	862.0
56.00	5488.0
57.00	8799.0
58.00	441.0
59.20	108.0
60.00	3121.0
61.00	16042.0
62.00	15183.0
63.00	12015.0
64.00	1130.0
65.00	473.0
67.00	850.0
68.00	29976.0
69.00	30624.0
70.00	2575.0
72.00	1765.0
73.00	14155.0
74.00	51208.0
75.00	145280.0
76.10	12740.0
77.00	1726.0
77.90	1151.0
78.90	12685.0
80.00	3216.0
81.00	12950.0
81.90	2845.0
82.90	263.0
85.80	192.0
87.00	10905.0
88.00	10382.0
90.90	1273.0
92.00	8682.0
93.00	11944.0
94.00	33752.0
95.10	250176.0
96.10	16600.0
97.00	479.0
103.00	227.0
103.90	1397.0
105.00	437.0
105.90	1153.0
106.90	363.0
109.90	200.0
110.90	344.0
112.00	254.0
112.90	293.0
115.00	269.0
115.90	1180.0
117.00	2006.0
117.90	1203.0
118.90	1576.0
123.90	202.0
125.90	123.0
127.90	1070.0
128.90	442.0
129.90	1003.0
131.00	396.0
135.00	567.0
135.80	105.0
137.00	650.0
140.10	250.0
141.00	3162.0
141.90	499.0
143.00	3308.0
143.90	276.0
145.00	242.0
145.90	351.0
147.00	194.0
147.90	653.0
148.90	198.0
149.90	302.0
152.90	141.0
154.20	151.0
154.90	447.0
155.80	105.0
156.90	395.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

159.00	290.0
160.90	287.0
169.40	246.0
170.80	285.0
171.40	437.0
172.10	1118.0
174.00	194880.0
175.10	15368.0
176.00	186048.0
177.00	12873.0
178.00	355.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	3029.0
37.00	16464.0
38.00	14562.0
39.10	4831.0
39.90	439.0
43.00	239.0
44.00	2914.0
45.00	2903.0
46.10	273.0
47.00	3400.0
48.00	1808.0
49.00	13699.0
50.00	58320.0
51.00	17424.0
52.00	811.0
55.00	764.0
56.00	5173.0
57.00	8200.0
58.00	430.0
60.00	2771.0
61.00	14978.0
62.00	14187.0
63.00	10892.0
64.00	1029.0
65.00	421.0
67.00	841.0
68.00	27960.0
69.00	28360.0
70.00	2392.0
72.00	1591.0
73.00	13159.0
74.00	47752.0
75.00	136064.0
76.00	11728.0
77.00	1549.0
78.00	1086.0
78.90	11713.0
80.00	3002.0
81.00	12012.0
81.90	2698.0
83.00	242.0
85.80	190.0
87.00	10123.0
88.00	9803.0
90.90	1187.0
92.00	7770.0
93.00	11353.0
94.00	31072.0
95.10	234304.0
96.10	15403.0
97.00	425.0
103.00	208.0
103.90	1279.0
104.90	363.0
105.90	1132.0
106.90	297.0
109.80	184.0
110.90	340.0
112.00	257.0
113.00	234.0
114.90	257.0
115.90	1072.0
117.00	2008.0
117.90	1152.0
118.90	1463.0
123.90	163.0
125.80	106.0
127.90	920.0
128.90	349.0
129.90	854.0
130.90	360.0
135.00	600.0
135.90	109.0
137.00	616.0
139.00	108.0
140.00	256.0
141.00	3108.0
141.90	437.0
143.00	3053.0
143.90	243.0
145.00	180.0
145.80	338.0
147.00	145.0
147.90	678.0
148.90	183.0
149.90	270.0
151.90	107.0
152.90	164.0
154.10	150.0
154.90	480.0
156.90	384.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

159.00	314.0
160.90	262.0
169.40	192.0
170.80	252.0
171.40	438.0
172.10	1073.0
173.20	3708.0
174.00	187328.0
175.00	14495.0
176.00	179328.0
177.00	11903.0
178.00	346.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12