

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU093020\
 Data File : VU040399.D
 Acq On : 30 Sep 2020 15:16
 Operator : SY/MD
 Sample : L4139-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG4A2

Quant Time: Oct 01 03:48:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 01 03:05:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	132676	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	124105	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	66472	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	26282	4.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.00%
7) Chloroethane-d5	1.92	69	26265	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.40%
11) 1,1-Dichloroethene-d2	2.58	63	42743	2.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.20%#
20) 2-Butanone-d5	4.65	46	151710	46.50	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.00%
24) Chloroform-d	5.08	84	69857	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	5.72	65	42769	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
32) Benzene-d6	5.75	84	120628	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	6.70	67	44220	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.91	98	92683	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.60%
43) trans-1,3-Dichloropropene-	8.19	79	15424	4.14	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.80%
46) 2-Hexanone-d5	8.64	63	102974	47.00	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.00%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	40608	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	49022	4.86	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.20%

Target Compounds

					Ovalue
3) Chloromethane	1.53	50	1226	0.094 ug/L	86
8) Chloroethane	1.94	64	7687	1.011 ug/L #	69
13) Acetone	2.66	43	3878	1.426 ug/L	73
17) Methyl tert-butyl Ether	3.38	73	11679	0.420 ug/L #	43
25) Chloroform	5.11	83	4271	0.195 ug/L	99
30) Cyclohexane	5.40	56	6399	0.365 ug/L	92
33) Benzene	5.79	78	5304826	127.494 ug/L	100
35) Methylcyclohexane	6.77	83	4101	0.253 ug/L	92
42) Toluene	7.98	91	14820	0.347 ug/L	97
51) Chlorobenzene	9.45	112	543651	19.708 ug/L	98
52) Ethylbenzene	9.57	91	128963	2.785 ug/L	100
53) m,p-Xylene	9.69	106	1188913	68.930 ug/L	99
54) o-Xylene	10.10	106	514500	31.708 ug/L	97
56) Isopropylbenzene	10.48	105	95744	2.187 ug/L	99
62) 1,3-Dichlorobenzene	11.74	146	2394	0.109 ug/L	96
63) 1,4-Dichlorobenzene	11.83	146	29528	1.290 ug/L	95
65) 1,2-Dichlorobenzene	12.20	146	8103	0.379 ug/L	91

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU093020\
Data File : VU040399.D
Acq On : 30 Sep 2020 15:16
Operator : SY/MD
Sample : L4139-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG4A2

Quant Time: Oct 01 03:48:20 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 01 03:05:40 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU093020\
Data File : VU040399.D
Acq On : 30 Sep 2020 15:16
Operator : SY/MD
Sample : L4139-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG4A2

Quant Time: Oct 01 03:48:20 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 01 03:05:40 2020
Response via : Initial Calibration

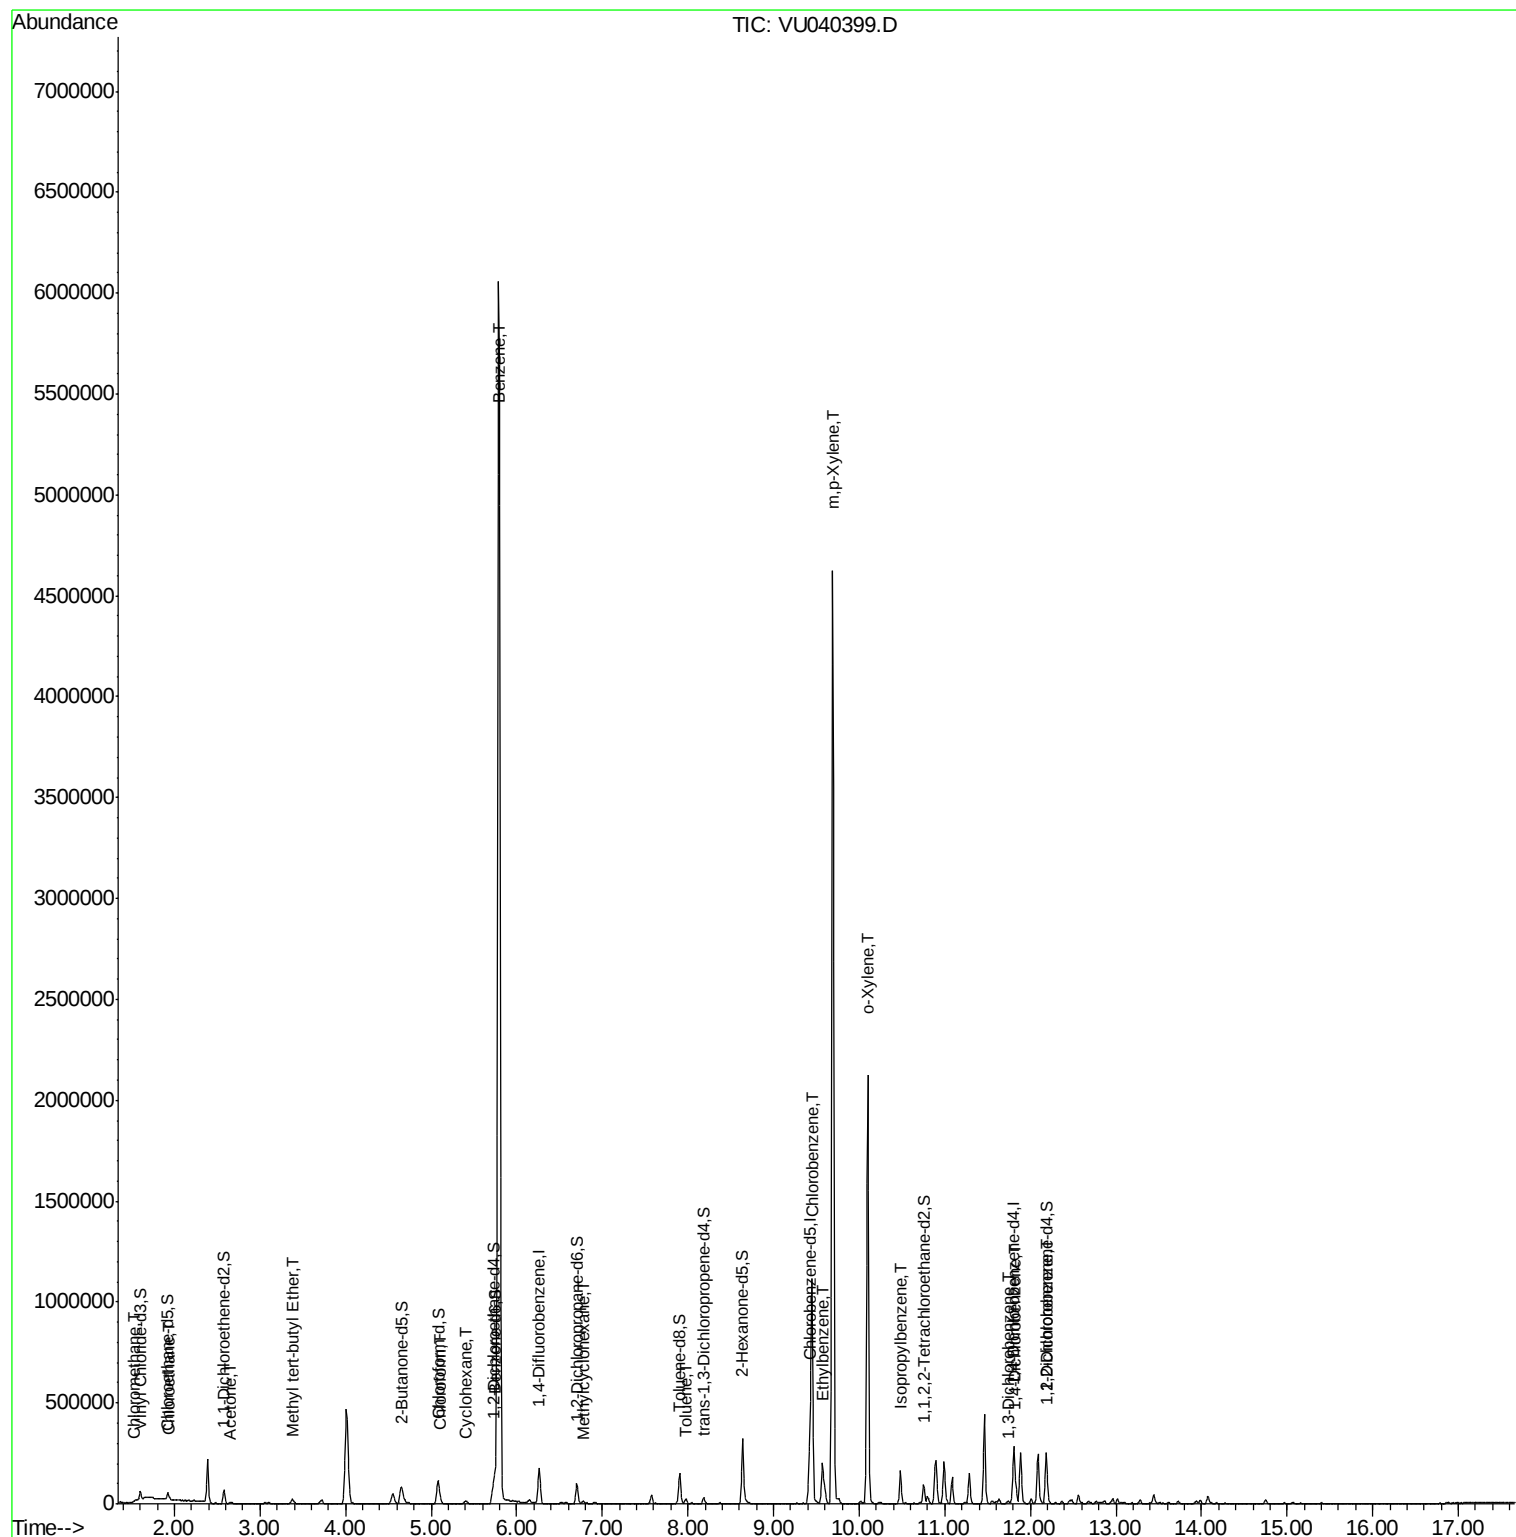



#3

Chloromethane

Concen: 0.094 ug/L

RT: 1.53 min Scan# 58

Delta R.T. 0.00 min

Lab File: VU040399.D

Acq: 30 Sep 2020 15:16

Instrument :

MSVOA_U

ClientSampled :


BG4A2

Tot Ion: 50 Resp: 1226

Ion Ratio Lower Upper


50 100

52 40.5 23.0 42.6





Abundance Ion 50.05 (49.75 to 50.75): VU0

Ion 52.05 (51.75 to 52.75): VU0

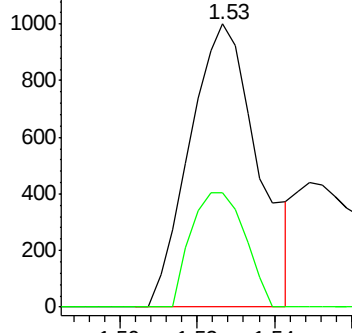

Time-->



#8

Chloroethane

Concen: 1.011 ug/L

RT: 1.94 min Scan# 188

Delta R.T. 0.00 min

Lab File: VU040399.D


Acq: 30 Sep 2020 15:16

Tgt Ion: 64 Resp: 7687

Ion Ratio Lower Upper


64 100

66 13.8 21.3 39.6#





Abundance Ion 64.10 (63.80 to 64.80): VU0

Ion 66.05 (65.75 to 66.75): VU0

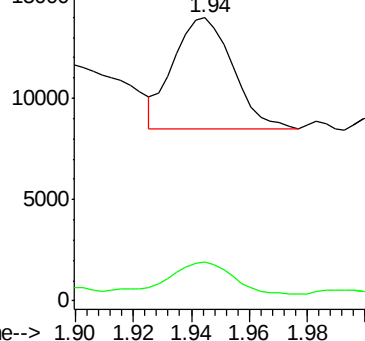

Time-->

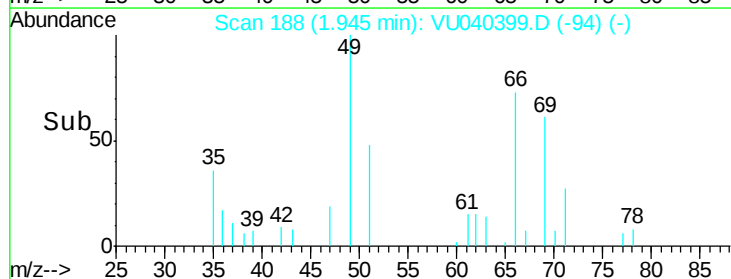

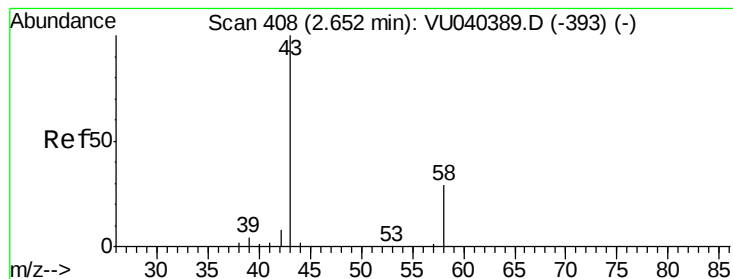

#13

Acetone

Concen: 1.426 ug/L

RT: 2.66 min Scan# 412

Delta R.T. 0.01 min

Lab File: VU040399.D

Acq: 30 Sep 2020 15:16

Instrument :

MSVOA_U

ClientSampled :


BG4A2

Tot Ion: 43 Resp: 3878

Ion Ratio Lower Upper

43 100

58 16.2 0.0 61.8

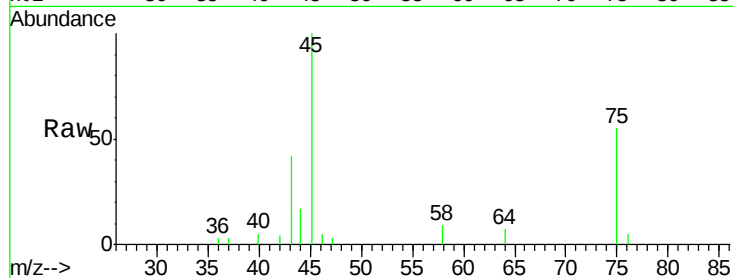

Abundance Ion 43.05 (42.75 to 43.75): VU040389.D (-393) (-)

Ion 58.05 (57.75 to 58.75): VU040389.D (-393) (-)

2.66

1500



1000

500

0

2.60 2.65 2.70 2.75

Time-->

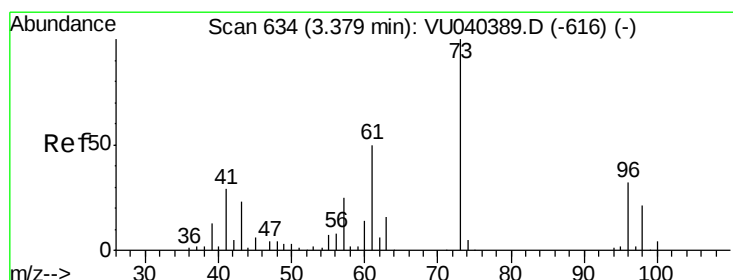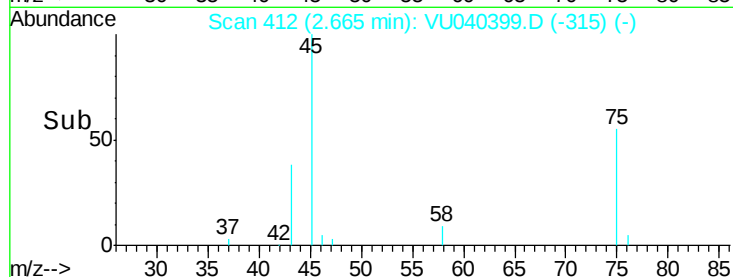

#17

Methyl tert-butyl Ether

Concen: 0.420 ug/L

RT: 3.38 min Scan# 634

Delta R.T. 0.00 min

Lab File: VU040399.D

Acq: 30 Sep 2020 15:16


Tgt Ion: 73 Resp: 11679

Ion Ratio Lower Upper

73 100

43 37.5 19.0 28.4#

57 66.2 18.9 28.3#

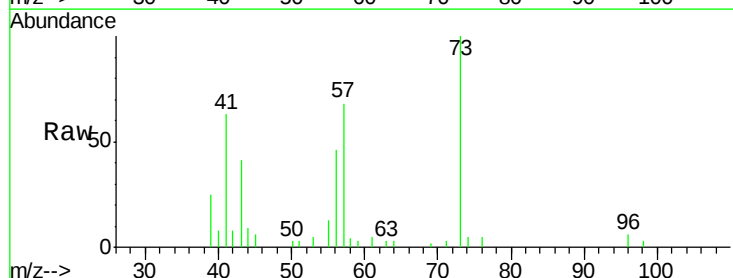

Abundance Ion 73.10 (72.80 to 73.80): VU040389.D (-616) (-)

Ion 43.05 (42.75 to 43.75): VU040389.D (-616) (-)

Ion 57.10 (56.80 to 57.80): VU040389.D (-616) (-)

3.38

6000


4000


2000

0

3.30 3.35 3.40 3.45

Time-->




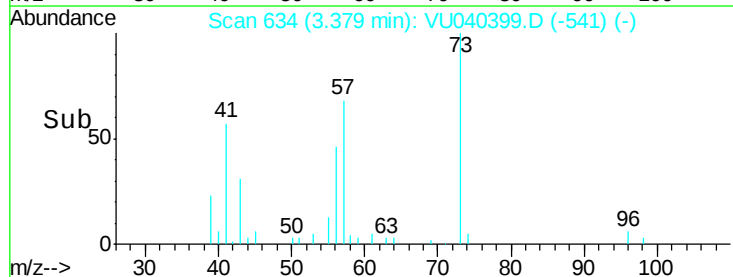


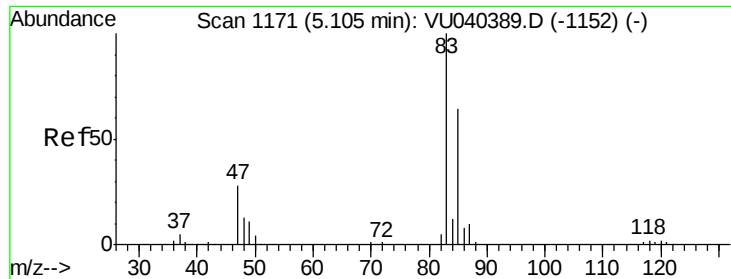

#25
Chloroform
Concen: 0.195 ug/L
RT: 5.11 min Scan# 1172
Delta R.T. 0.00 min
Lab File: VU040399.D
Acq: 30 Sep 2020 15:16




Instrument :
MSVOA_U
ClientSampled :
BG4A2


Tot Ion: 83 Resp: 4271
Ion Ratio Lower Upper
83 100
85 64.7 44.6 82.8

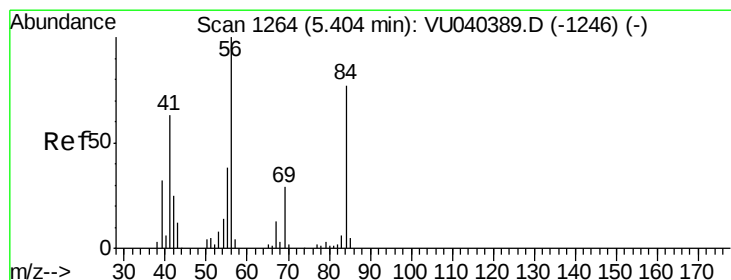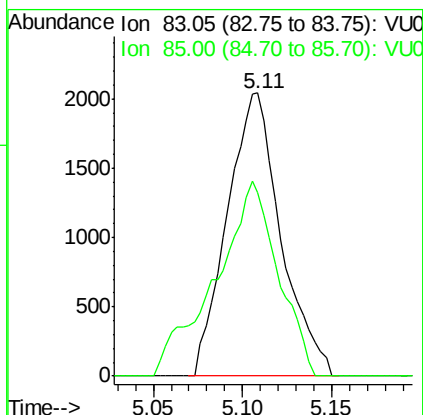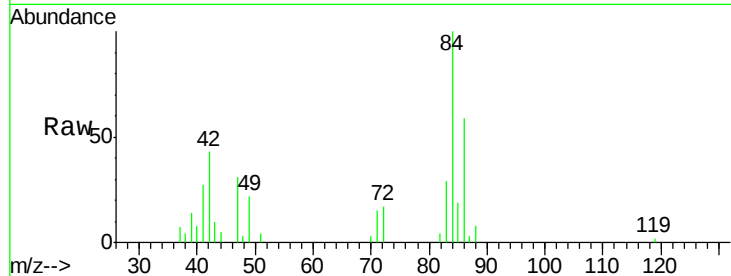

#30
Cyclohexane
Concen: 0.365 ug/L
RT: 5.40 min Scan# 1264
Delta R.T. 0.00 min
Lab File: VU040399.D
Acq: 30 Sep 2020 15:16

Tgt Ion: 56 Resp: 6399
Ion Ratio Lower Upper
56 100
69 32.3 23.3 34.9
84 88.2 64.2 96.4

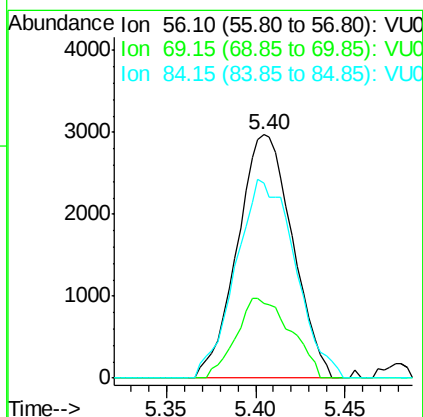

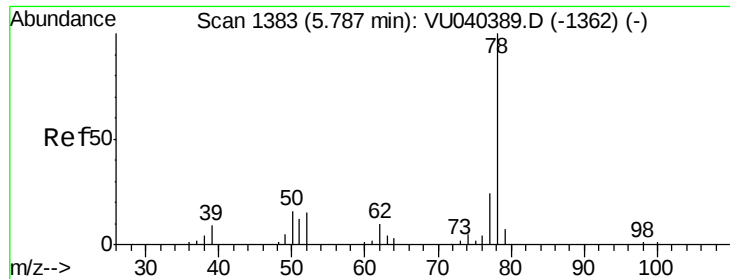

#33

Benzene

Concen: 127.494 ug/L

RT: 5.79 min Scan# 1384





Delta R.T. 0.00 min

Lab File: VU040399.D

Acq: 30 Sep 2020 15:16

Instrument :
MSVOA_U
ClientSampleId :
BG4A2

Tgt Ion: 78 Resp: 5304826

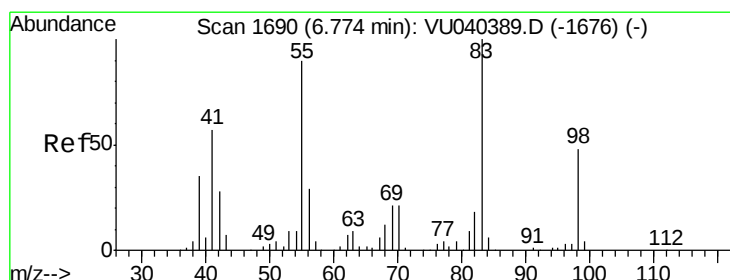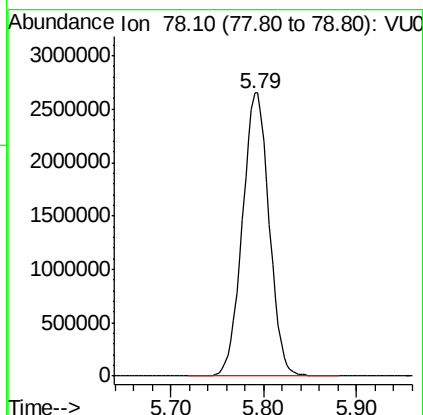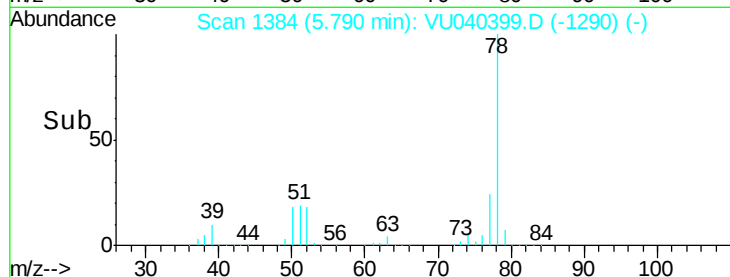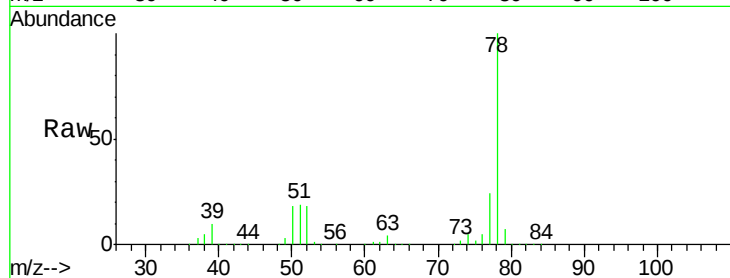

#35

Methylcyclohexane

Concen: 0.253 ug/L

RT: 6.77 min Scan# 1690

Delta R.T. 0.00 min

Lab File: VU040399.D




Acq: 30 Sep 2020 15:16


Tgt Ion: 83 Resp: 4101

Ion	Ratio	Lower	Upper
83	100		

55	98.3	71.4	107.2
----	------	------	-------

98	44.7	38.5	57.7
----	------	------	------

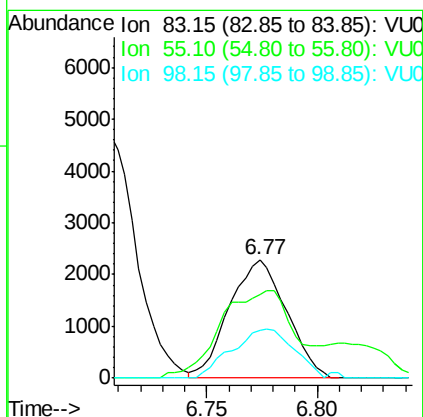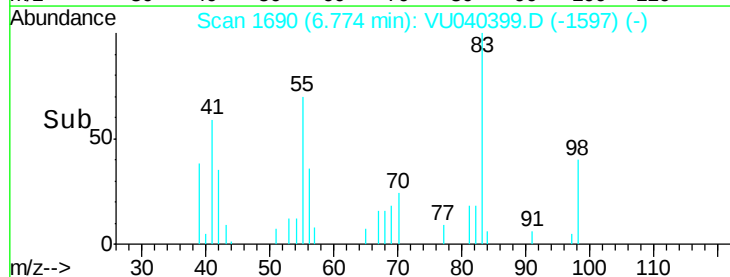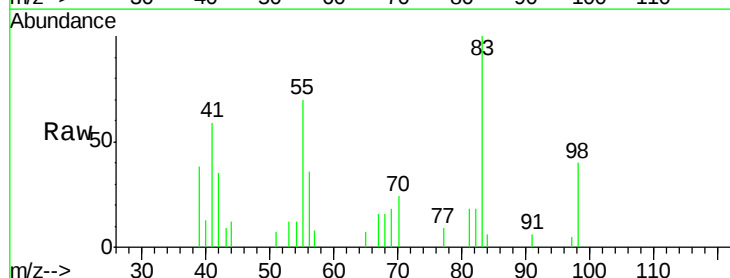

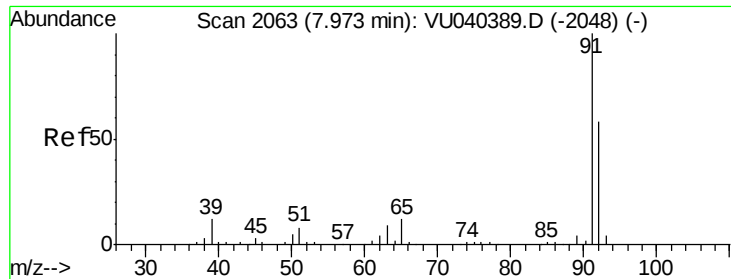

#42

Toluene

Concen: 0.347 ug/L

RT: 7.98 min Scan# 2064

Delta R.T. 0.00 min

Lab File: VU040399.D

Acq: 30 Sep 2020 15:16

Instrument :

MSVOA_U

ClientSampleId :


BG4A2

Tot Ion: 91 Resp: 14820

Ion Ratio Lower Upper




91 100

92 59.6 40.0 74.4

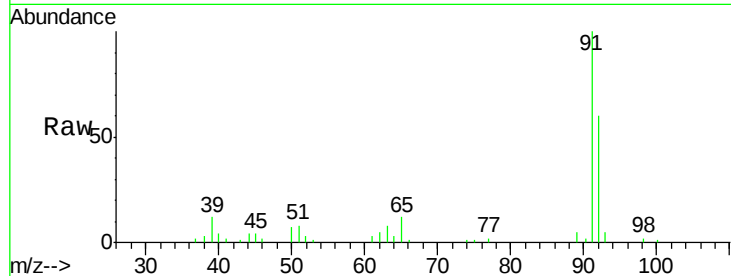

Abundance Ion 91.15 (90.85 to 91.85): VU0

Ion 92.15 (91.85 to 92.85): VU0

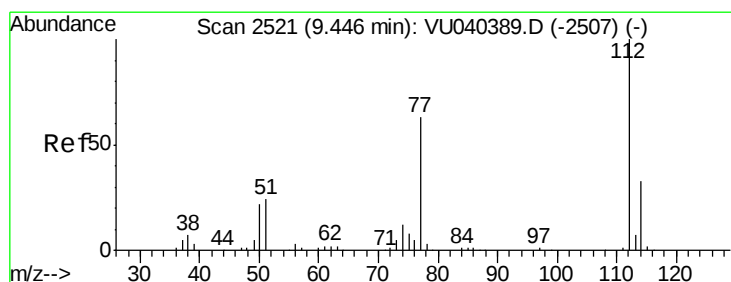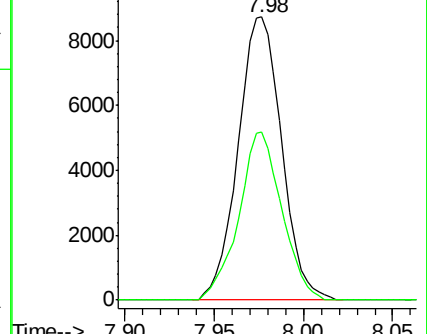

#51

Chlorobenzene

Concen: 19.708 ug/L

RT: 9.45 min Scan# 2522

Delta R.T. 0.00 min

Lab File: VU040399.D

Acq: 30 Sep 2020 15:16


Tgt Ion: 112 Resp: 543651

Ion Ratio Lower Upper

112 100

114 32.3 22.0 40.8



77 63.6 49.5 74.3




Abundance Ion 112.10 (111.80 to 112.80): V

Ion 114.05 (113.75 to 114.75): V

Ion 77.10 (76.80 to 77.80): VU0




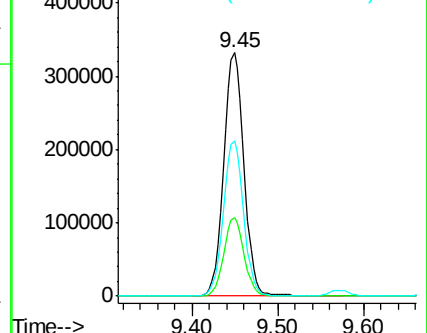


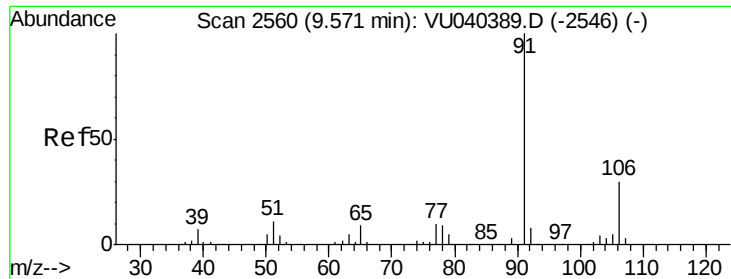

#52
Ethylbenzene
Concen: 2.785 ug/L
RT: 9.57 min Scan# 2560
Delta R.T. 0.00 min
Lab File: VU040399.D
Acq: 30 Sep 2020 15:16




Instrument :
MSVOA_U
ClientSampled :
BG4A2


Tot Ion: 91 Resp: 128963
Ion Ratio Lower Upper
91 100
106 30.2 21.1 39.3

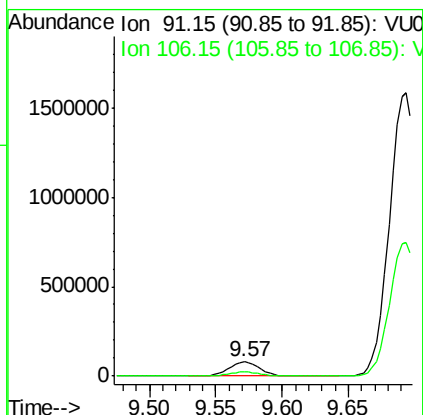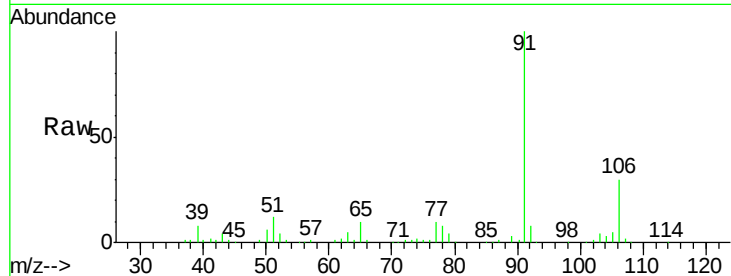

#53
m,p-Xylene
Concen: 68.930 ug/L
RT: 9.69 min Scan# 2598
Delta R.T. 0.00 min
Lab File: VU040399.D
Acq: 30 Sep 2020 15:16

Tgt Ion: 106 Resp: 1188913
Ion Ratio Lower Upper
106 100
91 211.0 149.0 276.6

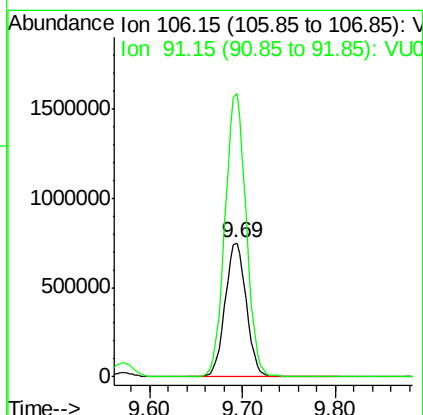


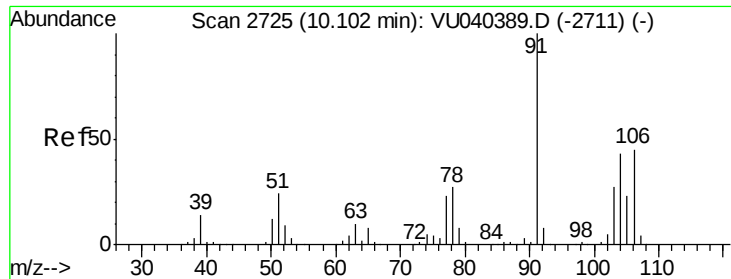




#54
o-Xylene
Concen: 31.708 ug/L
RT: 10.10 min Scan# 2724
Delta R.T. -0.00 min
Lab File: VU040399.D
Acq: 30 Sep 2020 15:16

Instrument :
MSVOA_U
ClientSampled :
BG4A2

Tot Ion:106 Resp: 514500
Ion Ratio Lower Upper
106 100
91 225.5 160.9 298.9

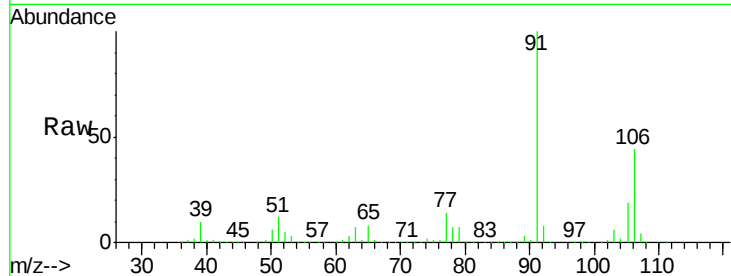


Abundance Ion 106.15 (105.85 to 106.85): V
Ion 91.15 (90.85 to 91.85): VU0


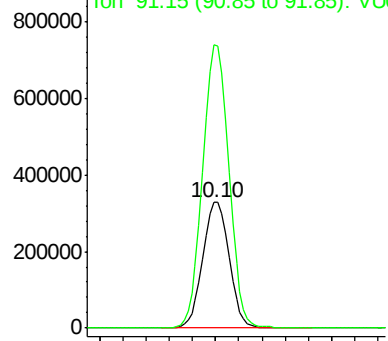



#56
Isopropylbenzene
Concen: 2.187 ug/L
RT: 10.48 min Scan# 2843
Delta R.T. -0.00 min
Lab File: VU040399.D
Acq: 30 Sep 2020 15:16

Tgt Ion:105 Resp: 95744
Ion Ratio Lower Upper
105 100
120 26.4 20.6 30.8
77 17.8 14.3 21.5



Abundance Ion 105.05 (104.75 to 105.75): V
Ion 120.10 (119.80 to 120.80): V
Ion 77.10 (76.80 to 77.80): VU0

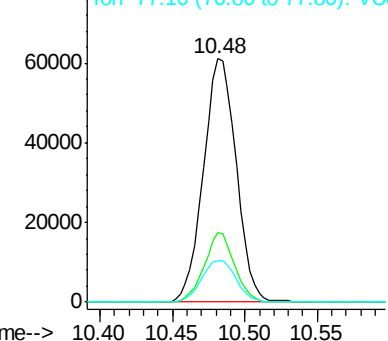

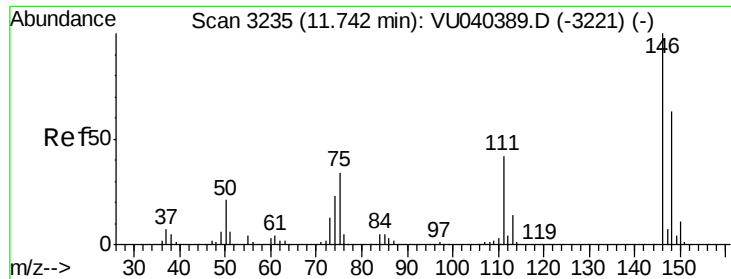

#62

1,3-Dichlorobenzene

Concen: 0.109 ug/L

RT: 11.74 min Scan# 3235

Delta R.T. 0.00 min

Lab File: VU040399.D

Acq: 30 Sep 2020 15:16

Instrument :

MSVOA_U

ClientSampled :

BG4A2


Tot Ion:146 Resp: 2394

Ion Ratio Lower Upper

146 100

111 41.8 28.6 53.0




148 57.4 43.4 80.6

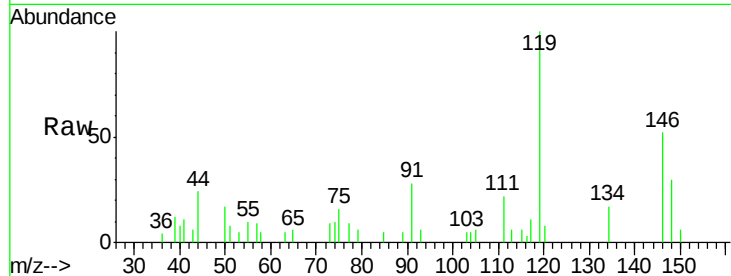

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

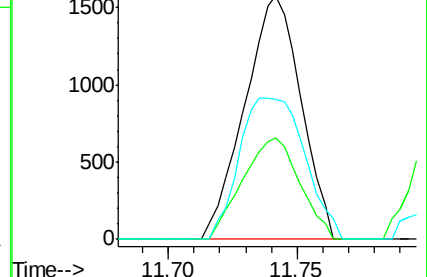

#63

1,4-Dichlorobenzene

Concen: 1.290 ug/L

RT: 11.83 min Scan# 3263

Delta R.T. 0.00 min

Lab File: VU040399.D

Acq: 30 Sep 2020 15:16


Tgt Ion:146 Resp: 29528

Ion Ratio Lower Upper

146 100

111 42.4 29.2 54.2



148 68.8 44.4 82.4




Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

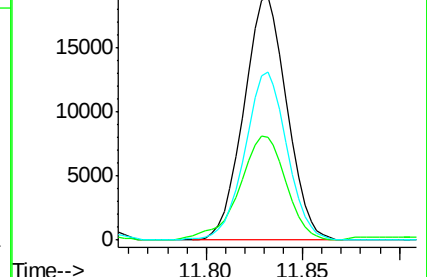


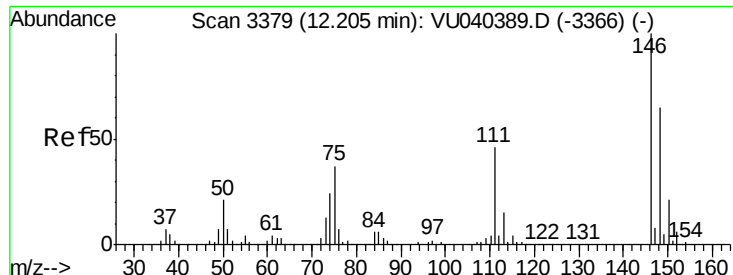

#65
 1,2-Dichlorobenzene
 Concen: 0.379 ug/L
 RT: 12.20 min Scan# 3379
 Delta R.T. 0.00 min
 Lab File: VU040399.D
 Acq: 30 Sep 2020 15:16

Instrument :
 MSVOA_U
 ClientSampleId :
 BG4A2

Tot Ion:146 Resp: 8103
 Ion Ratio Lower Upper
 146 100
 111 47.2 35.6 53.4
 148 71.5 49.8 74.6

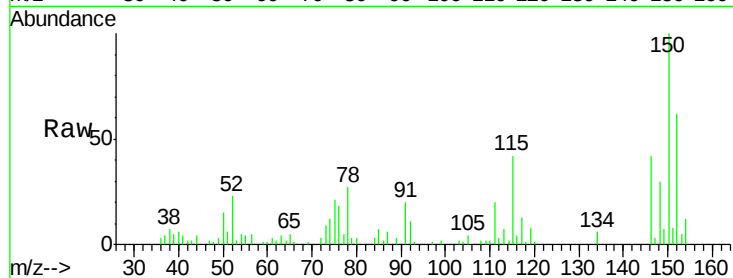

Abundance Ion 145.95 (145.65 to 146.65): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V

