


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU093020\
Data File : VU040388.D
Acq On : 30 Sep 2020 08:55
Operator : SY/MD
Sample : BFB10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB10

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Oct 01 03:05:40 2020

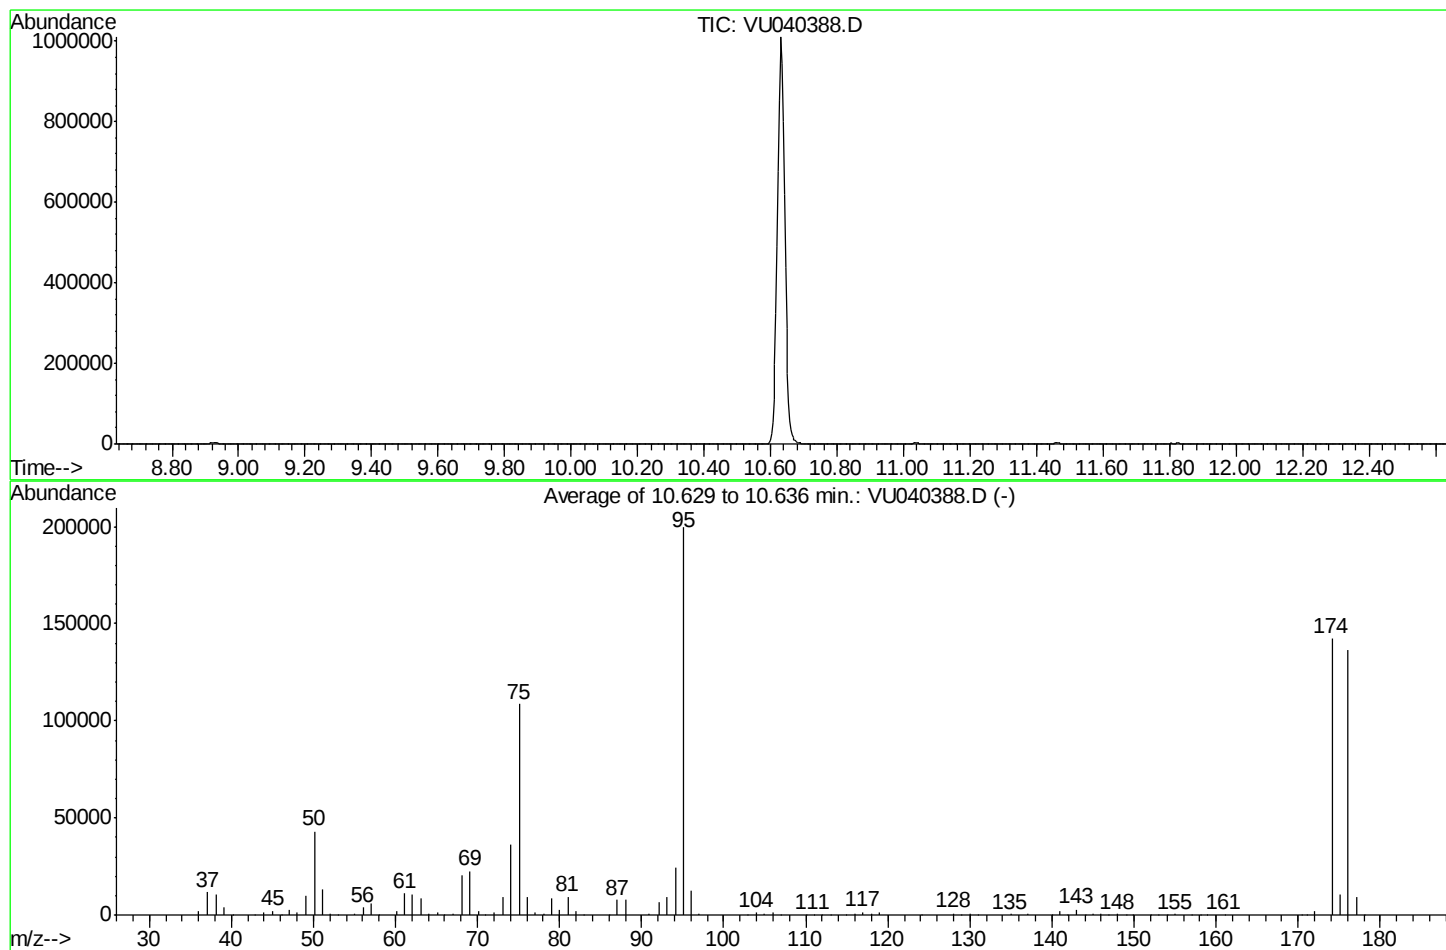

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	43069	PASS
75	95	30	80	54.5	108714	PASS
95	95	100	100	100.0	199658	PASS
96	95	5	9	6.2	12439	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.2	142250	PASS
175	174	5	9	7.4	10483	PASS
176	174	95	101	96.1	136704	PASS
177	176	5	9	6.6	9025	PASS

m/z	Abundance
36.00	2310.0
37.10	12274.0
38.10	11053.0
39.10	4491.0
40.20	268.0
42.90	135.0
44.00	1785.0
45.00	2115.0
46.00	246.0
47.10	2744.0
48.00	1393.0
49.10	10041.0
50.10	42928.0
51.10	13269.0
52.00	522.0
53.00	151.0
55.10	614.0
56.10	3779.0
57.10	6289.0
57.90	230.0
60.10	2304.0
61.10	11612.0
62.10	11014.0
63.10	8715.0
64.10	1122.0
65.10	1514.0
66.00	134.0
67.10	604.0
68.10	21488.0
69.10	22904.0
70.10	1607.0
72.00	1215.0
73.10	9071.0
74.10	36984.0
75.10	109416.0
76.10	9576.0
77.00	1276.0
78.10	767.0
79.00	9073.0
80.00	2508.0
81.00	9598.0
82.00	2243.0
82.90	155.0
86.10	243.0
87.10	8069.0
88.00	7806.0
91.00	902.0
92.10	6594.0
93.10	9079.0
94.10	24736.0
95.10	198976.0
96.10	12764.0
97.00	457.0
104.00	1026.0
104.90	404.0
106.00	1037.0
106.90	189.0
110.00	124.0
110.90	243.0
112.00	193.0
113.00	257.0
114.90	193.0
116.00	929.0
117.00	1381.0
118.00	976.0
119.00	1347.0
124.10	129.0
128.10	674.0
129.00	336.0
130.00	676.0
130.90	354.0
135.00	479.0
137.10	356.0
140.10	149.0
141.00	2230.0
141.90	246.0
143.00	2912.0
144.10	192.0
144.90	544.0
146.00	330.0
146.90	115.0
148.00	552.0
149.00	120.0
149.90	181.0
151.90	131.0
152.90	108.0
155.00	533.0
157.00	289.0
158.90	141.0
161.00	249.0
170.30	112.0
171.00	254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

172.10	1961.0
174.10	138176.0
175.10	10145.0
176.10	133568.0
177.10	9048.0
178.10	234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.00	2333.0
37.10	12261.0
38.10	10747.0
39.10	4468.0
40.10	289.0
42.90	147.0
44.00	1916.0
45.10	2115.0
46.10	276.0
47.10	2969.0
48.00	1397.0
49.10	10177.0
50.10	44496.0
51.10	13720.0
52.00	539.0
52.90	108.0
55.00	630.0
56.10	4027.0
57.10	6448.0
58.00	250.0
60.10	2328.0
61.10	11432.0
62.10	11170.0
63.10	8621.0
64.10	1031.0
65.10	1288.0
65.90	106.0
67.00	619.0
68.10	21240.0
69.10	23472.0
70.10	1807.0
70.90	101.0
72.00	1155.0
73.10	9355.0
74.10	37544.0
75.10	112632.0
76.10	9851.0
77.00	1416.0
78.10	726.0
79.00	9177.0
80.00	2452.0
81.00	9822.0
82.00	2335.0
82.90	198.0
86.00	218.0
87.10	8126.0
88.00	8093.0
91.00	916.0
92.10	6604.0
93.10	9545.0
94.10	25568.0
95.10	206976.0
96.10	12824.0
97.00	402.0
103.00	102.0
104.00	1083.0
104.90	423.0
105.90	1091.0
106.90	219.0
110.00	163.0
110.90	243.0
112.00	241.0
112.90	306.0
114.90	222.0
116.00	900.0
117.00	1399.0
118.00	989.0
119.00	1423.0
128.00	794.0
129.00	329.0
130.00	802.0
130.90	313.0
135.00	481.0
137.00	412.0
140.10	170.0
141.00	2381.0
142.00	245.0
143.00	3003.0
144.10	146.0
145.00	477.0
146.00	369.0
146.90	106.0
148.00	565.0
149.00	126.0
149.90	191.0
152.00	151.0
155.00	624.0
157.00	364.0
158.90	116.0
161.00	203.0
170.40	139.0
171.00	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

172.10	1823.0
174.10	147328.0
175.10	10770.0
176.10	141056.0
177.10	9367.0
178.10	226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.00	2152.0
37.10	10930.0
38.10	9646.0
39.10	3905.0
40.10	270.0
42.90	145.0
44.00	1916.0
45.10	1956.0
46.00	280.0
47.10	2730.0
48.00	1238.0
49.10	9410.0
50.10	41784.0
51.10	12885.0
52.00	530.0
52.90	115.0
55.00	549.0
56.10	3749.0
57.10	6030.0
58.00	227.0
60.10	2131.0
61.10	10186.0
62.10	10288.0
63.10	7905.0
64.10	859.0
65.10	1118.0
67.10	559.0
68.10	19360.0
69.10	21528.0
70.10	1713.0
70.90	109.0
72.00	996.0
73.10	9069.0
74.10	34496.0
75.10	104096.0
76.10	9050.0
77.00	1321.0
78.00	699.0
79.00	8492.0
80.00	2214.0
81.00	8998.0
82.00	2117.0
82.90	208.0
87.00	7521.0
88.00	7622.0
90.90	816.0
92.10	5898.0
93.10	8753.0
94.10	23704.0
95.10	193024.0
96.10	11729.0
97.00	299.0
102.90	142.0
104.00	1018.0
105.00	383.0
105.90	988.0
106.90	207.0
110.00	145.0
111.00	223.0
112.00	232.0
112.90	296.0
114.90	226.0
116.00	778.0
117.00	1372.0
118.00	906.0
119.00	1294.0
128.00	825.0
129.00	267.0
130.00	792.0
130.90	250.0
134.90	420.0
137.00	415.0
140.00	155.0
141.00	2241.0
142.00	265.0
143.00	2800.0
144.00	118.0
145.00	390.0
146.00	372.0
148.00	490.0
149.00	111.0
149.90	176.0
152.00	146.0
154.00	118.0
155.00	577.0
157.00	401.0
158.10	110.0
158.90	116.0
161.00	156.0
171.00	195.0
172.00	1556.0
174.10	141248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

175.10	10534.0
176.10	135488.0
177.10	8660.0
178.00	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

Scan 2875 (10.584 min): VU040388.D
BFB10

m/z	Abundance
39.90	157.0
44.00	450.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10