


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093021\
Data File : VU045034.D
Acq On : 30 Sep 2021 09:30
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
Title : SW846 8260
Last Update : Tue Sep 28 12:32:13 2021

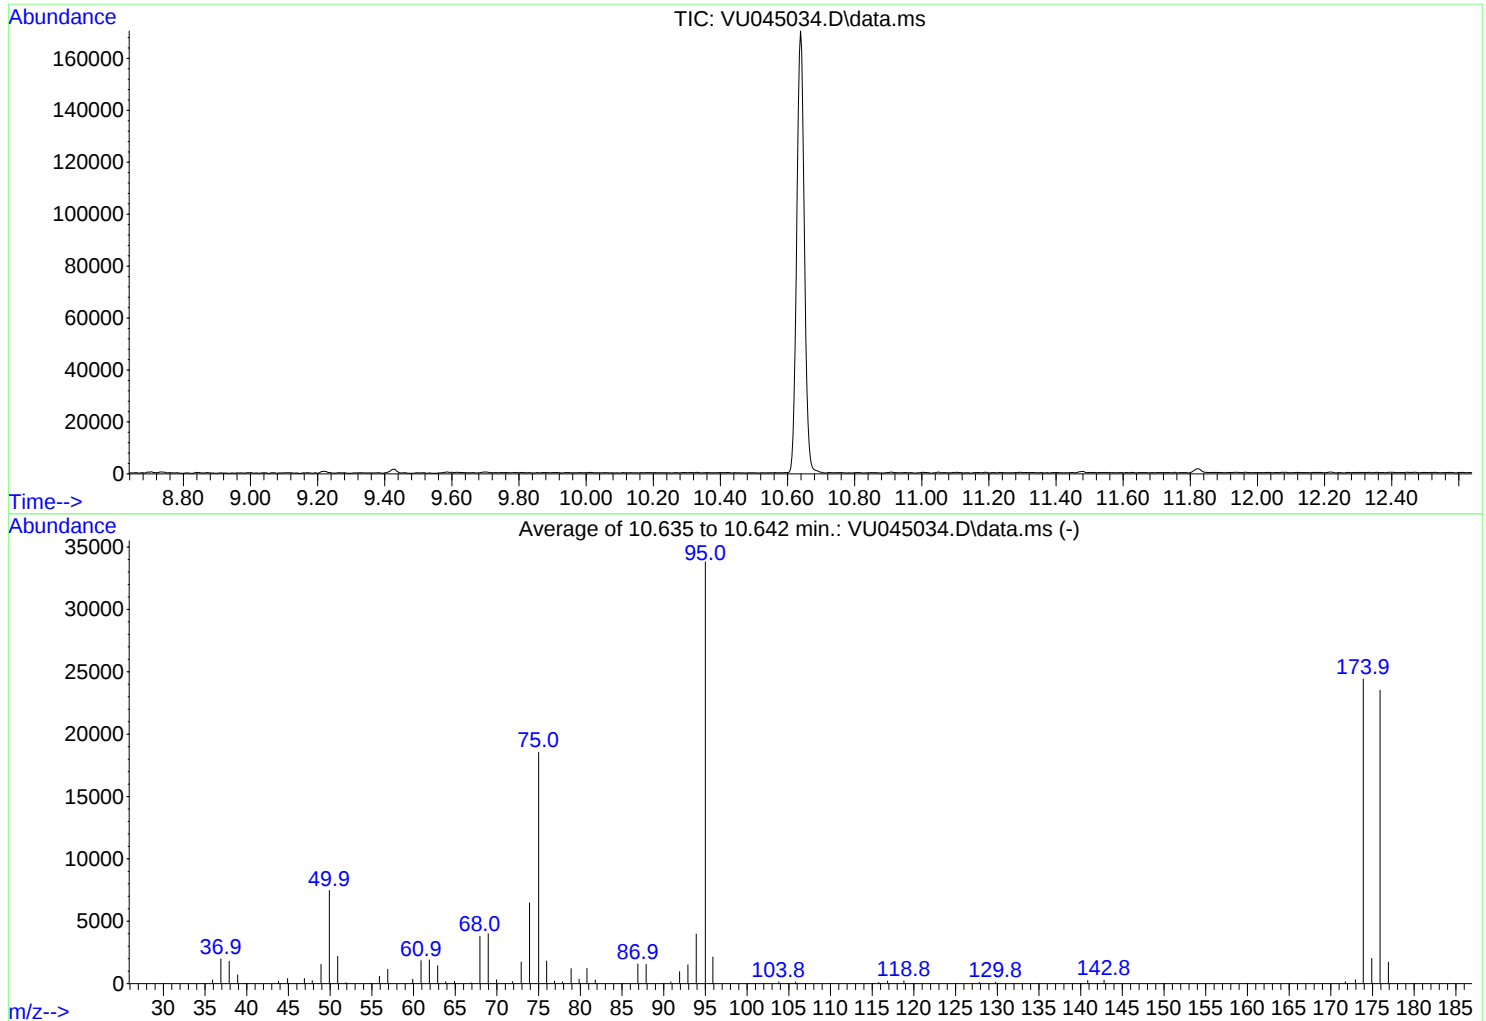

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.1	7469	PASS
75	95	30	60	54.8	18541	PASS
95	95	100	100	100.0	33811	PASS
96	95	5	9	6.3	2133	PASS
173	174	0.00	2	1.3	311	PASS
174	95	50	100	72.2	24419	PASS
175	174	5	9	8.3	2022	PASS
176	174	95	101	96.4	23528	PASS
177	176	5	9	7.3	1728	PASS