



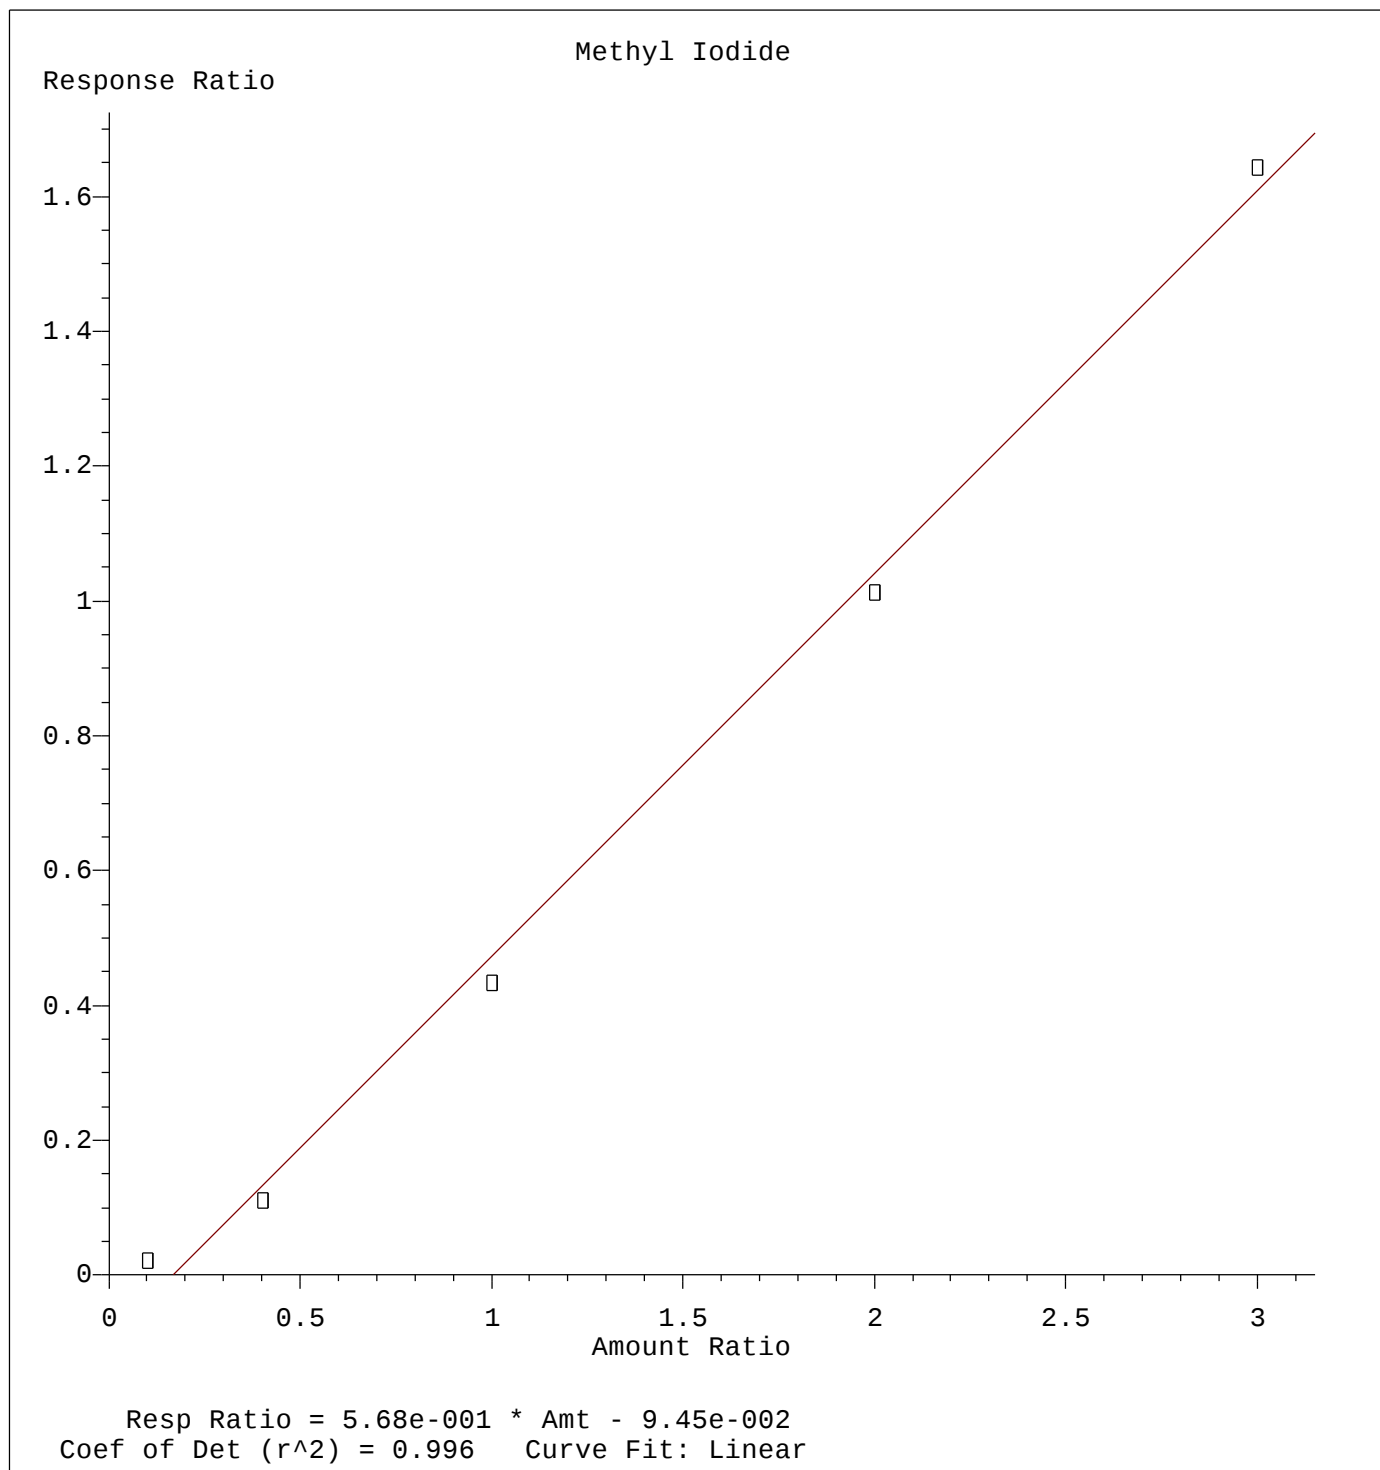

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Calibration Table Last Updated: Tue Oct 02 02:04:34 2018


Naphthalene

Response Ratio

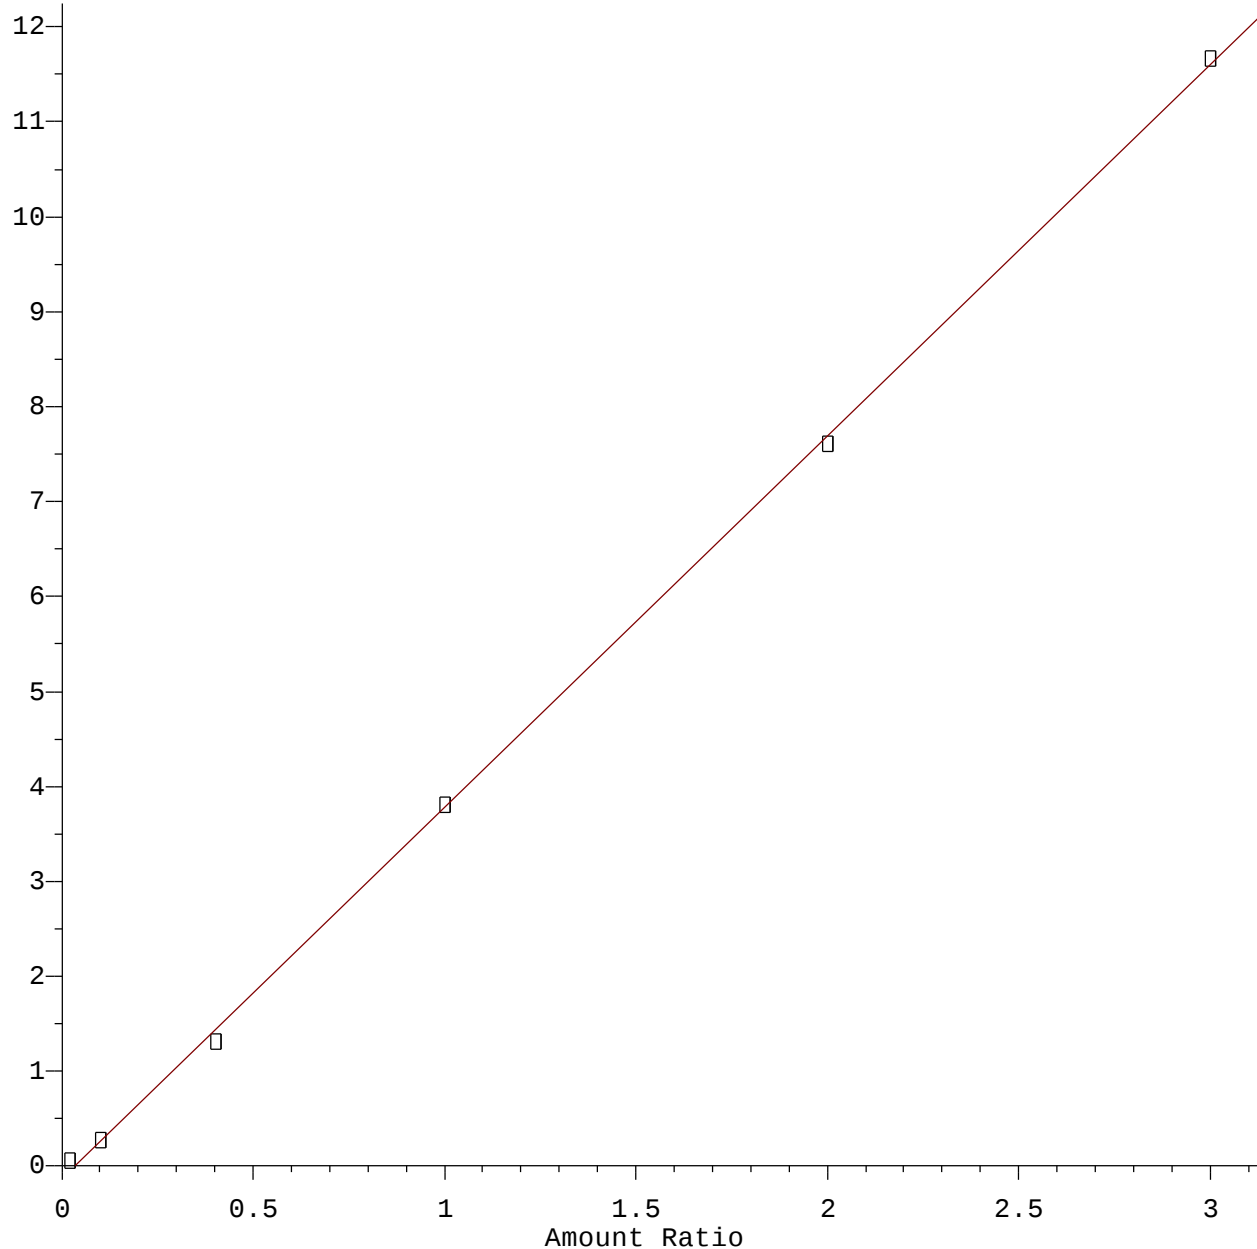


Resp Ratio = 3.91e+000 * Amt - 1.30e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Calibration Table Last Updated: Tue Oct 02 02:04:34 2018

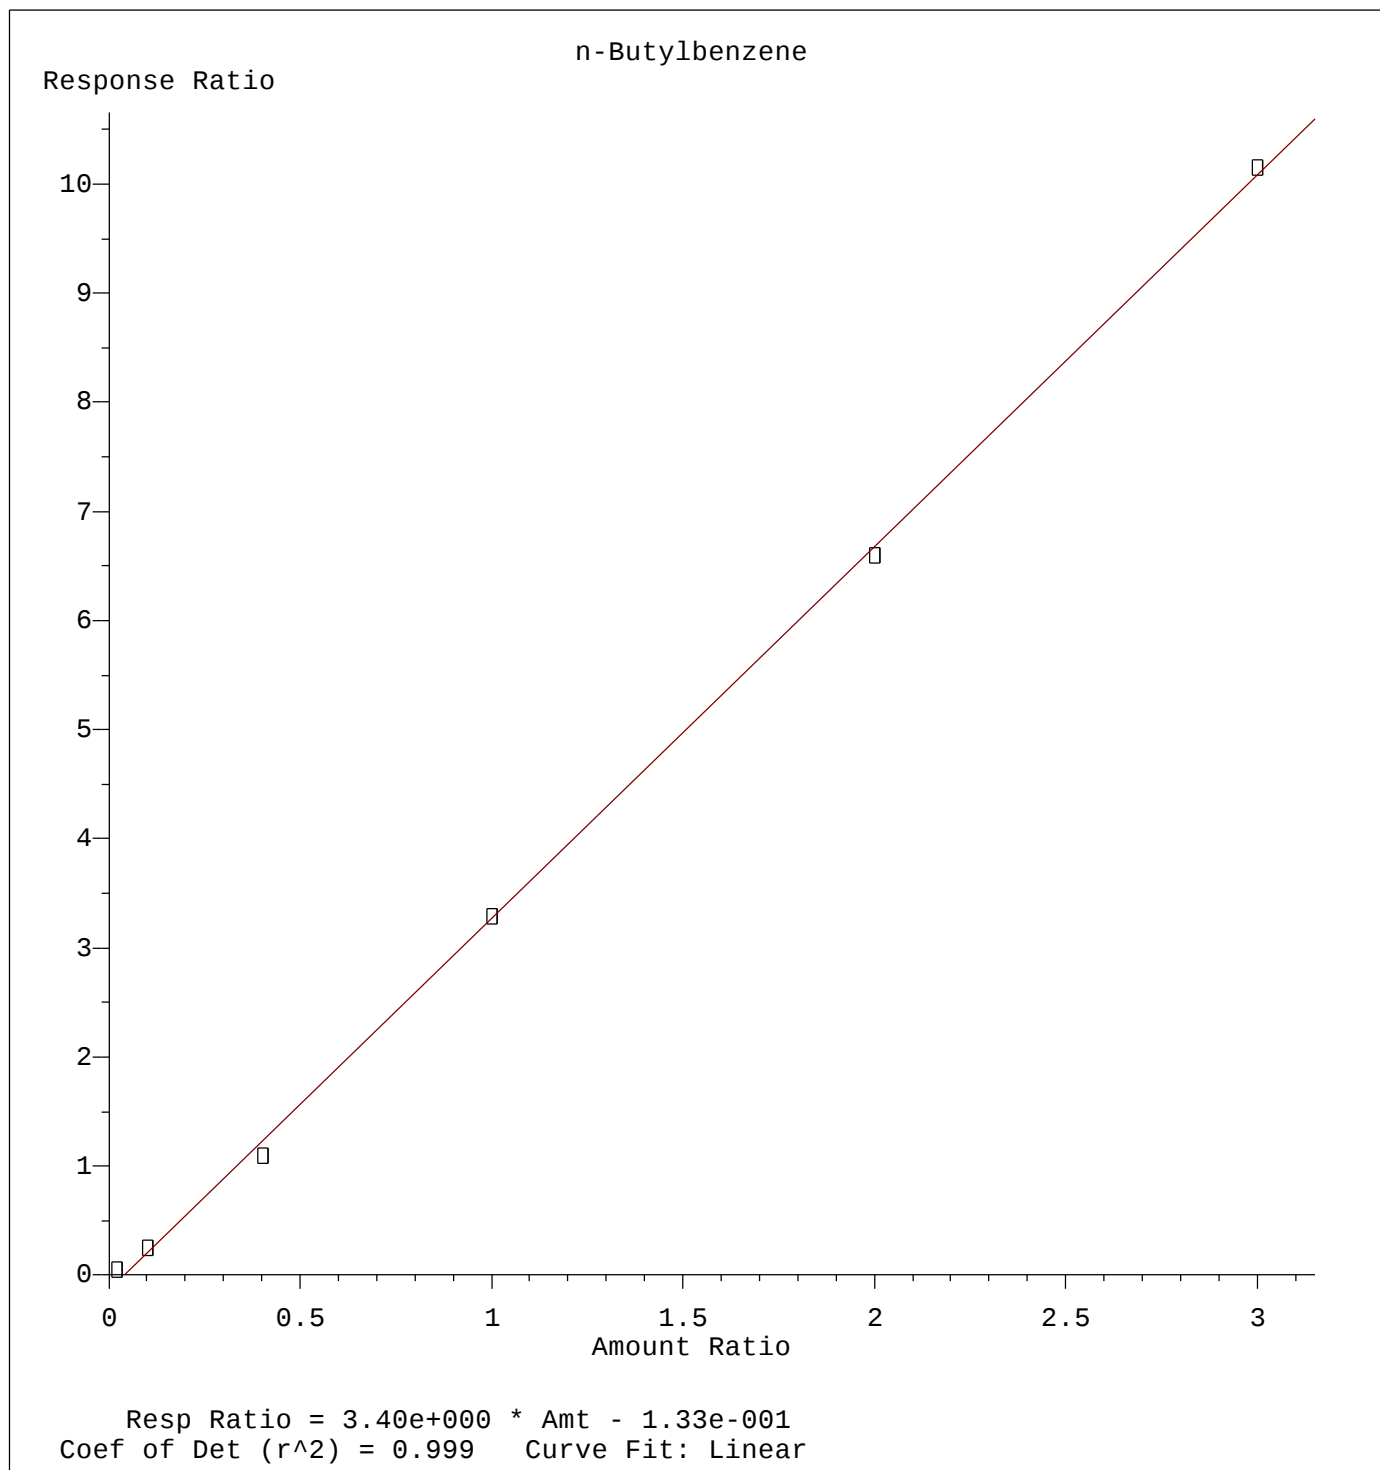


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Calibration Table Last Updated: Tue Oct 02 02:04:34 2018

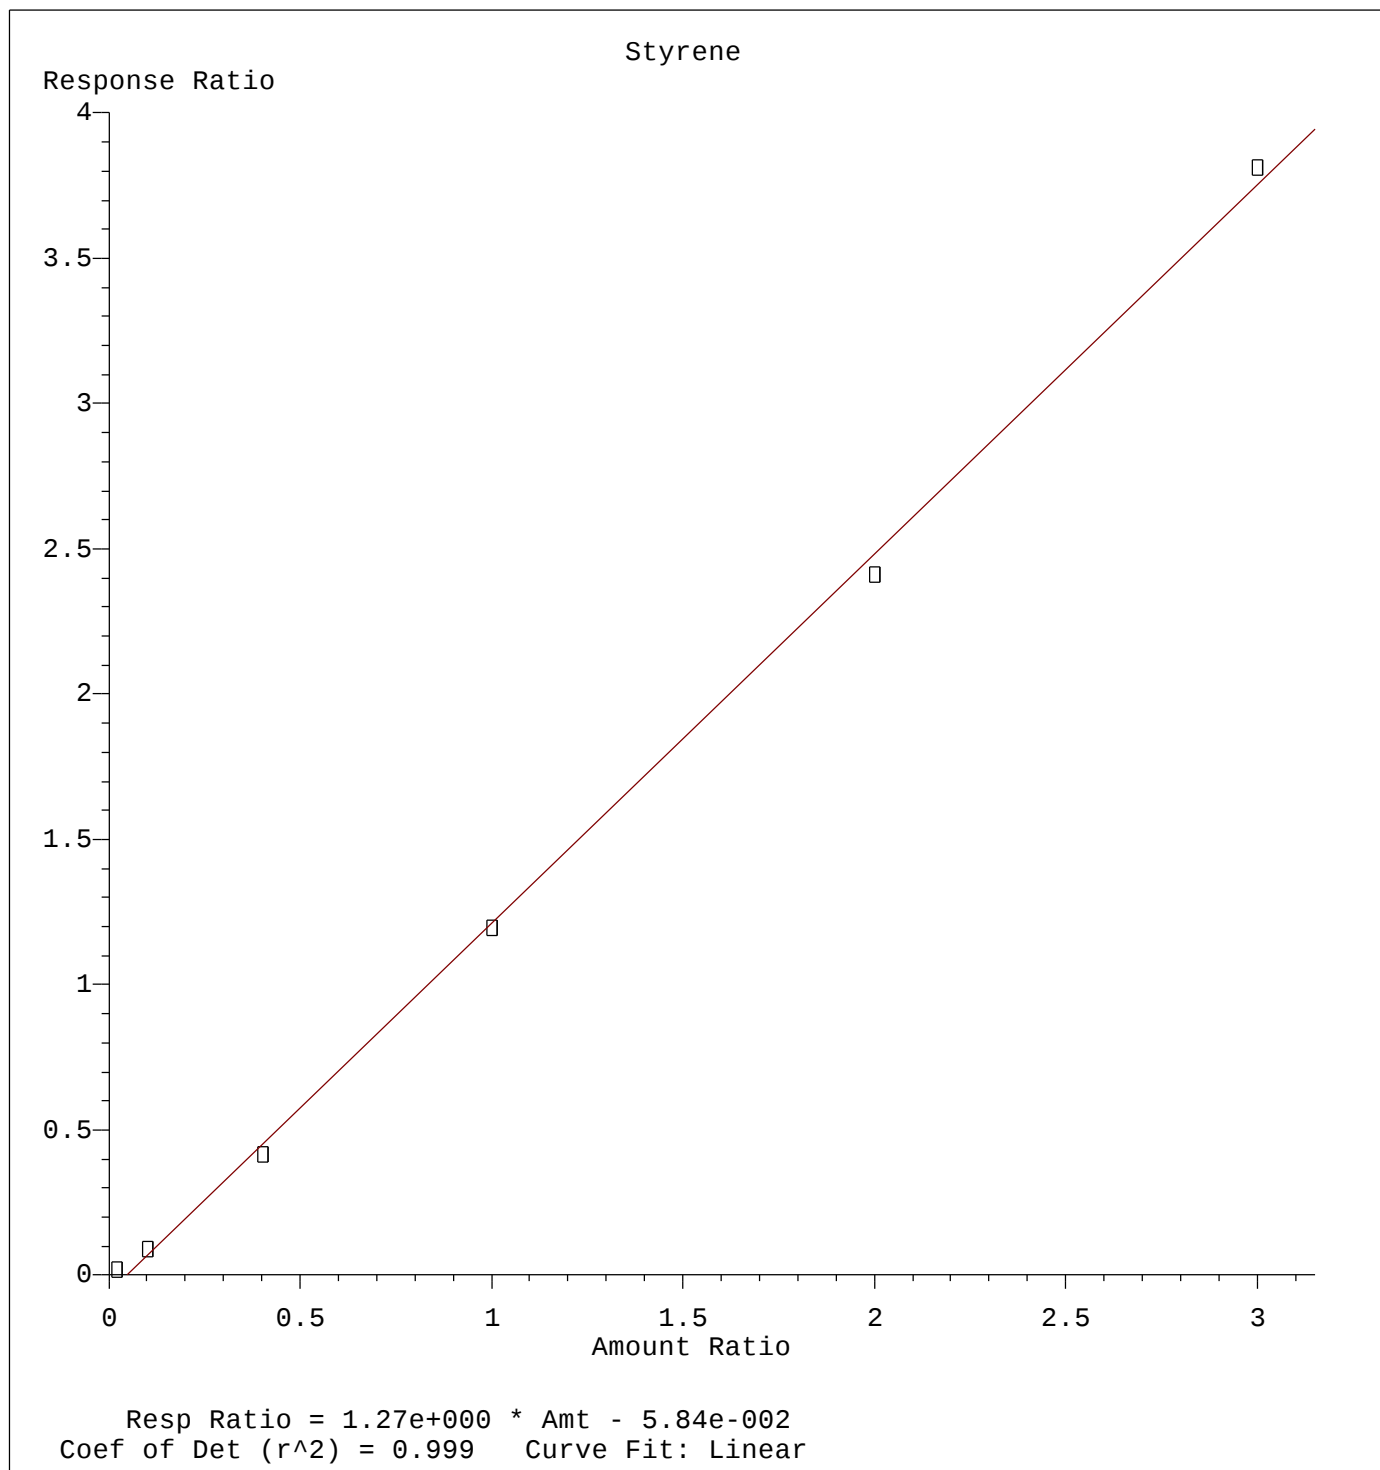

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Calibration Table Last Updated: Tue Oct 02 02:04:34 2018

2-Chloroethyl Vinyl ether

Response Ratio

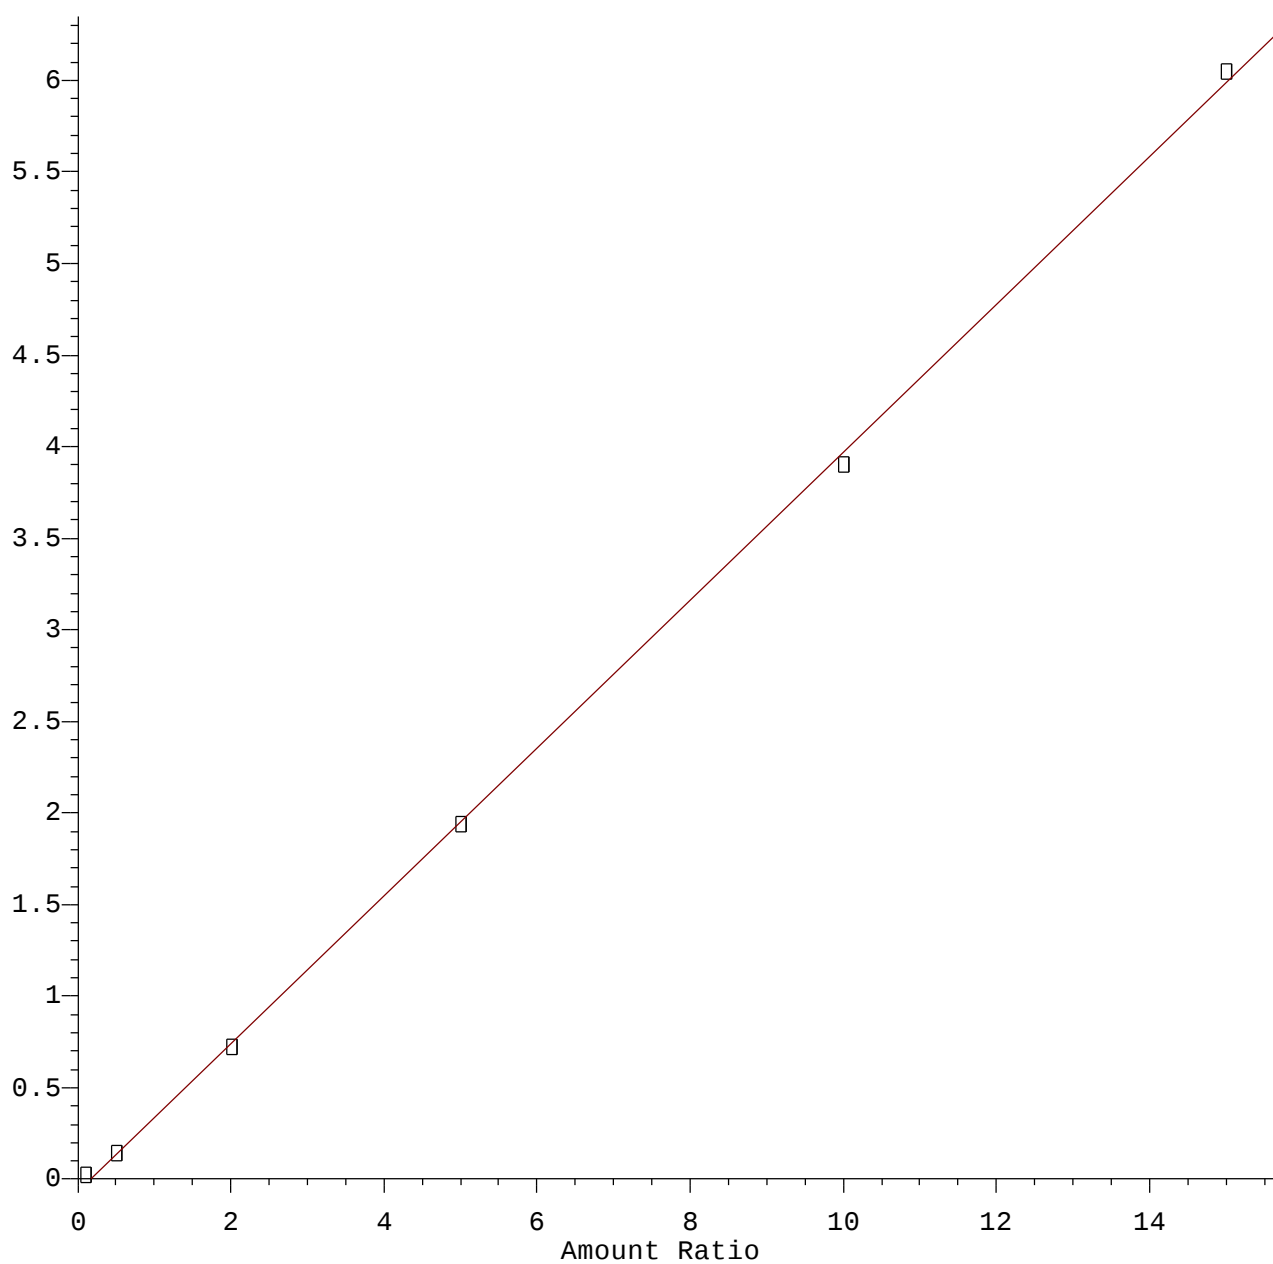


Resp Ratio = $4.04 \times 10^{-1} \times \text{Amt} - 6.64 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Calibration Table Last Updated: Tue Oct 02 02:04:34 2018


Ethyl methacrylate

Response Ratio

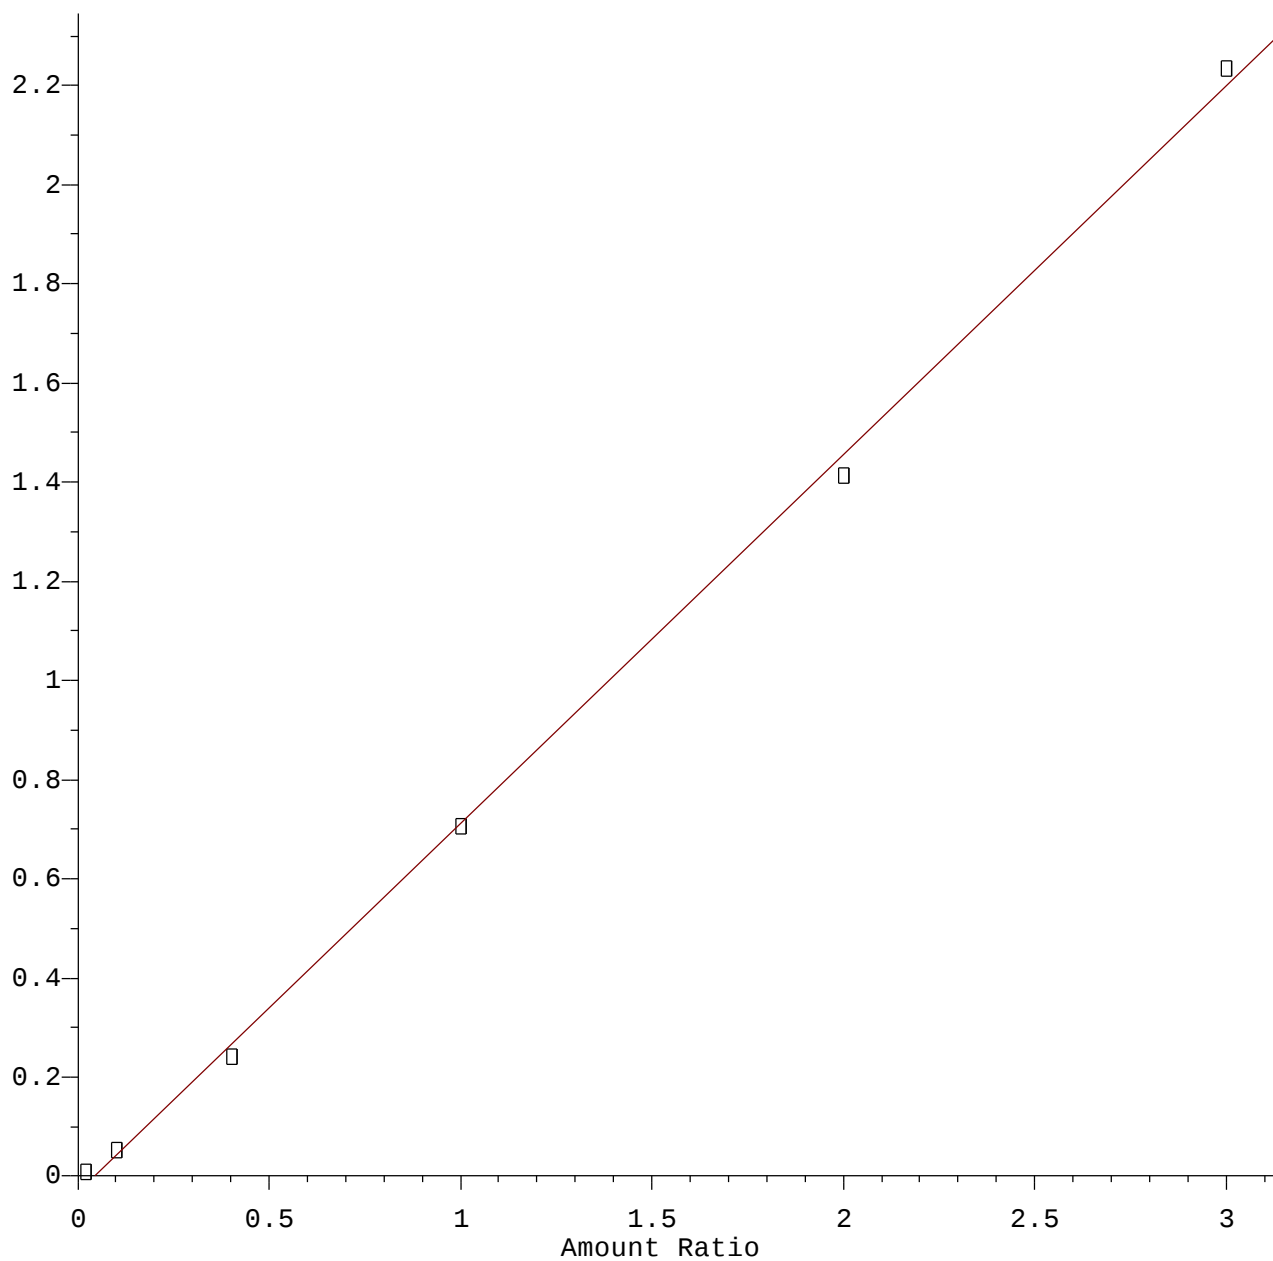

Resp Ratio = $7.44 \times 10^{-1} \times \text{Amt} - 3.38 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Calibration Table Last Updated: Tue Oct 02 02:04:34 2018

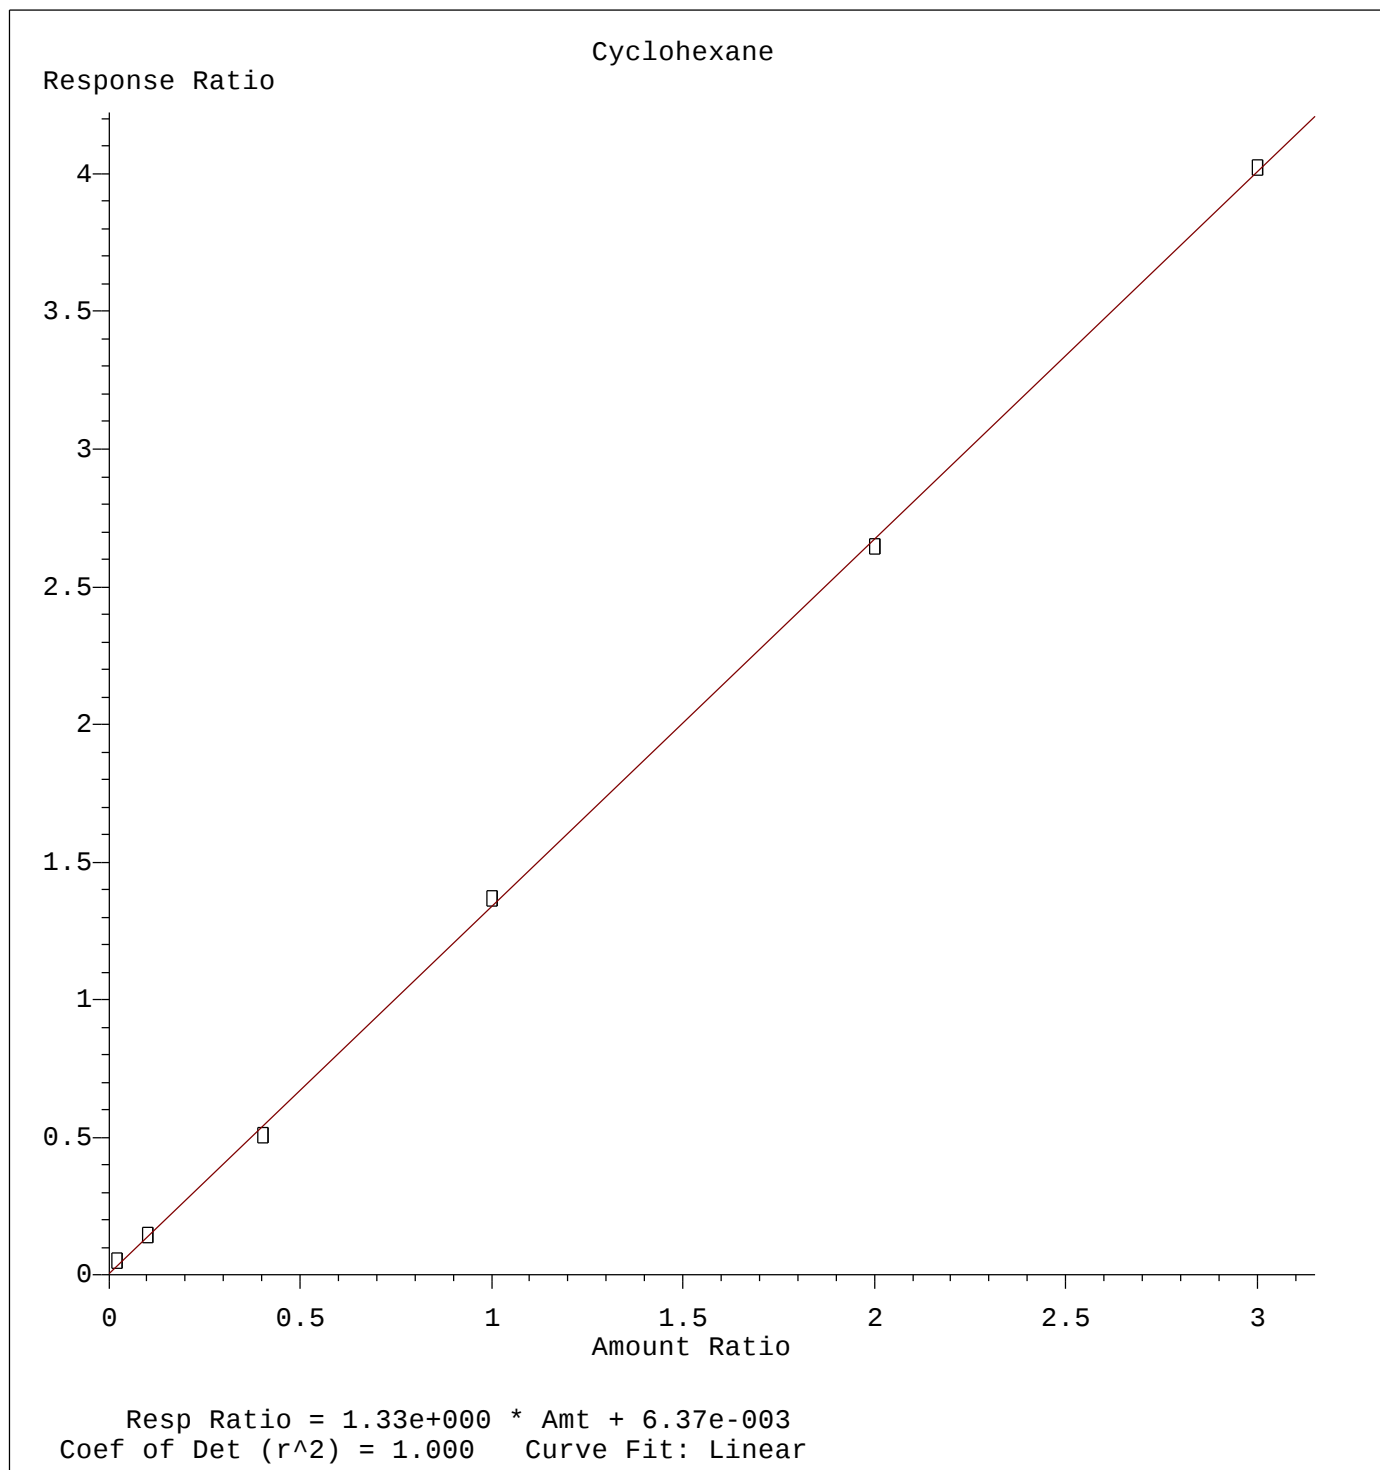

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Calibration Table Last Updated: Tue Oct 02 02:04:34 2018