


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100118\
Data File : VU027310.D
Acq On : 01 Oct 2018 09:19
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Title : SW846 8260
Last Update : Tue Oct 02 02:04:34 2018

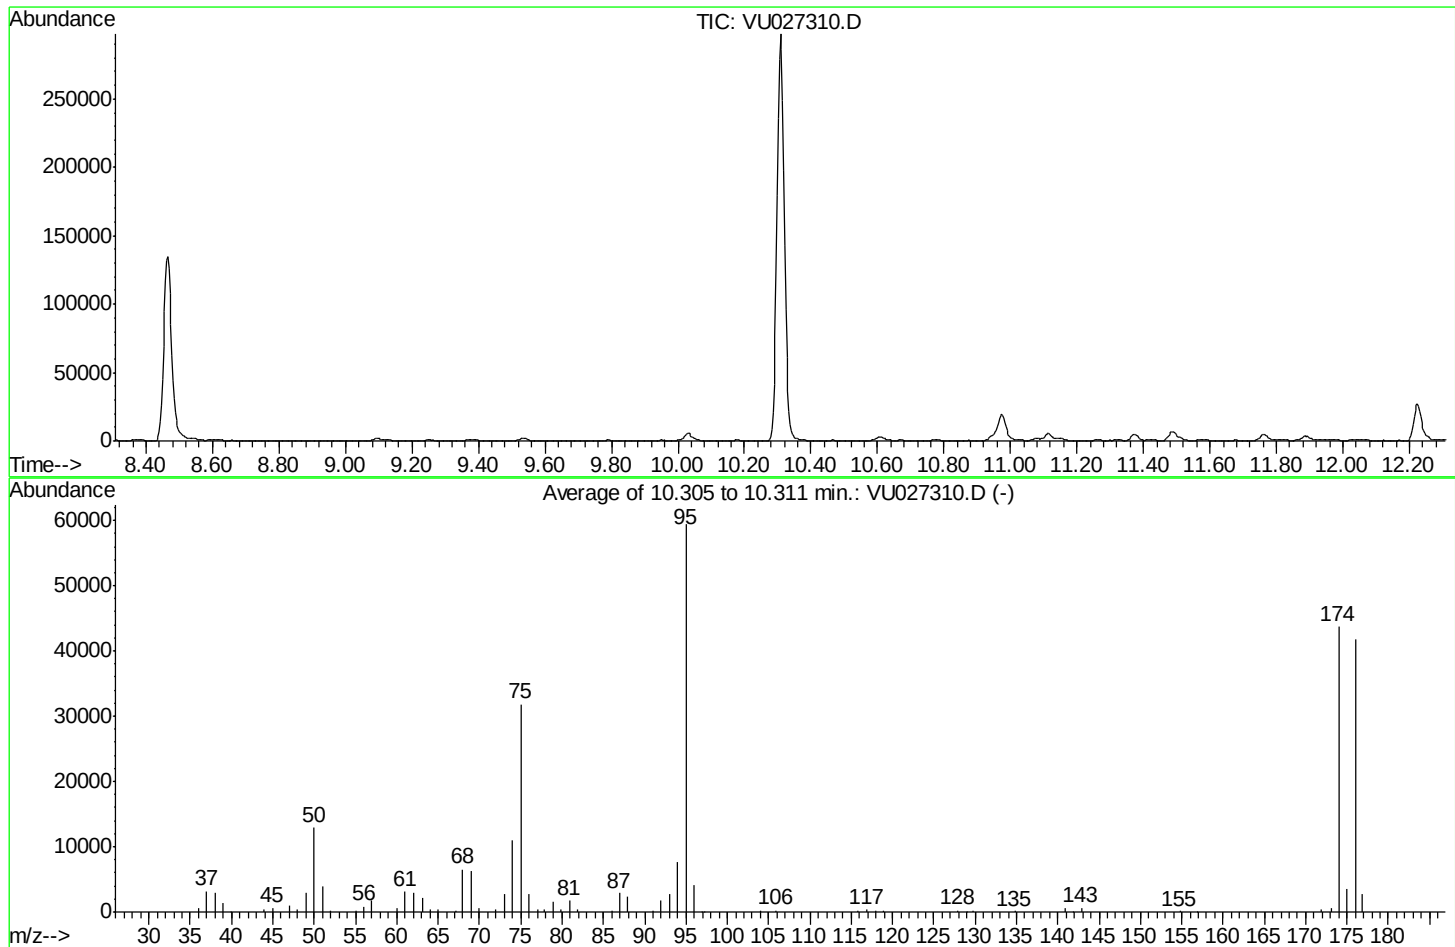

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	12920	PASS
75	95	30	60	53.6	31813	PASS
95	95	100	100	100.0	59400	PASS
96	95	5	9	6.9	4121	PASS
173	174	0.00	2	1.6	687	PASS
174	95	50	100	73.6	43720	PASS
175	174	5	9	8.1	3536	PASS
176	174	95	101	95.5	41760	PASS
177	176	5	9	6.5	2734	PASS