


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100119\
 Data File : VU034882.D
 Acq On : 30 Sep 2019 16:28
 Operator : JC/SP
 Sample : BFB40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB40

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100119WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 02 01:50:17 2019

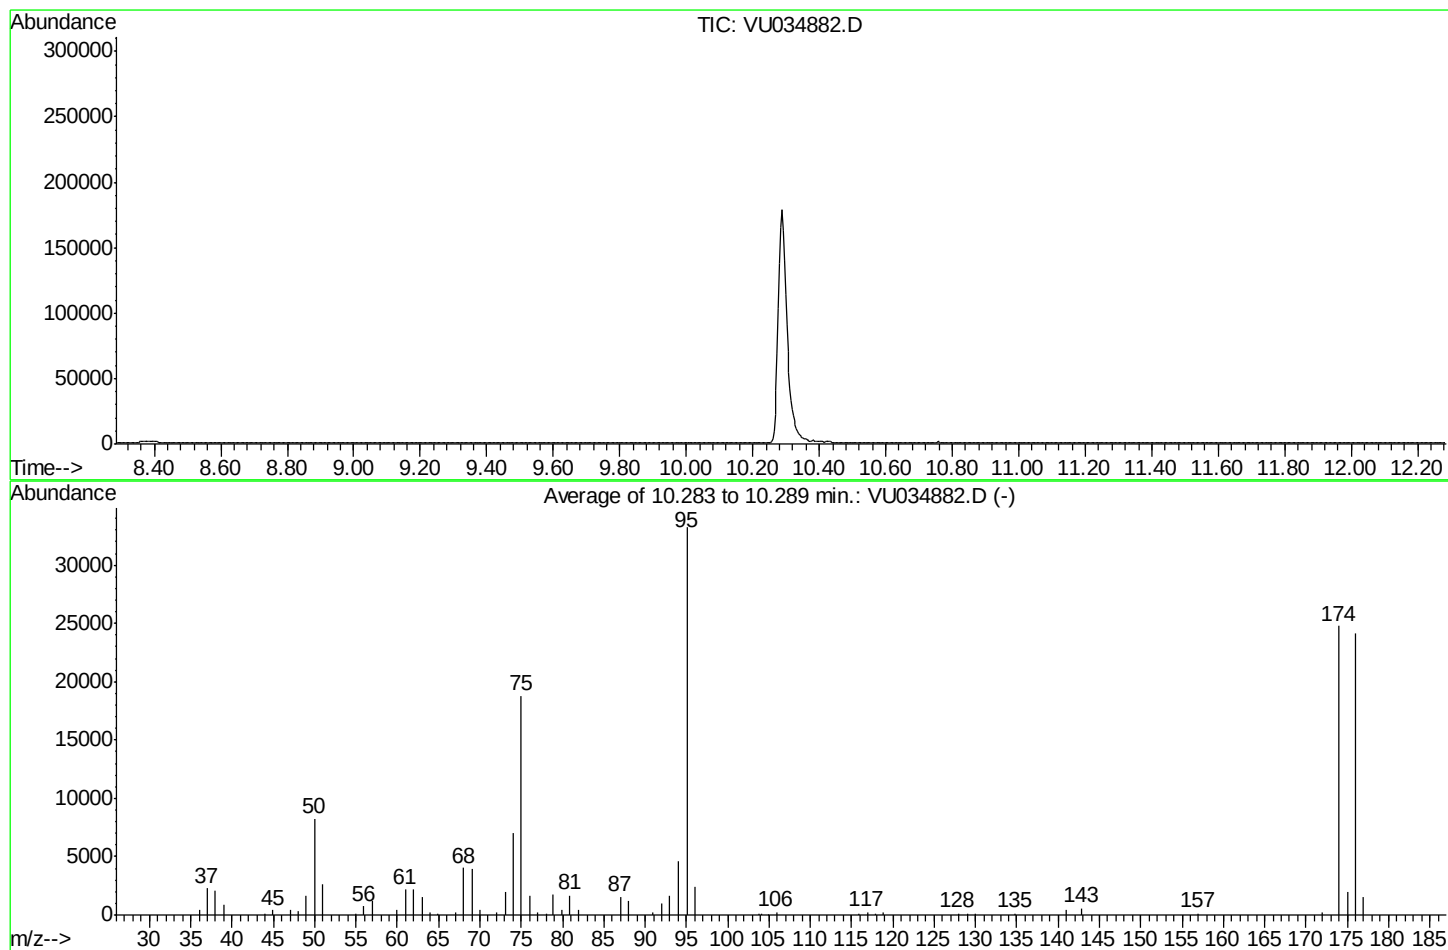

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	8251	PASS
75	95	30	80	56.5	18778	PASS
95	95	100	100	100.0	33234	PASS
96	95	5	9	7.4	2454	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.6	24784	PASS
175	174	5	9	8.2	2029	PASS
176	174	95	101	97.3	24104	PASS
177	176	5	9	6.5	1573	PASS

m/z	Abundance
36.00	510.0
37.00	2202.0
38.00	1902.0
39.00	780.0
39.90	247.0
44.00	829.0
44.90	388.0
47.00	492.0
48.00	314.0
49.00	1608.0
50.00	7919.0
51.00	2563.0
55.00	138.0
56.00	713.0
57.00	1309.0
59.90	421.0
61.00	2000.0
62.00	2193.0
63.00	1561.0
63.90	183.0
65.00	121.0
67.00	170.0
68.00	3909.0
69.00	3737.0
70.00	426.0
72.00	238.0
73.00	1995.0
74.10	6497.0
75.00	17800.0
76.10	1529.0
77.00	327.0
78.10	174.0
78.90	1648.0
79.90	476.0
80.90	1570.0
81.90	433.0
87.10	1469.0
88.00	1230.0
90.90	234.0
92.00	997.0
93.00	1517.0
94.00	4079.0
95.10	31528.0
96.00	2620.0
104.10	134.0
105.90	189.0
115.90	130.0
116.90	285.0
118.00	169.0
118.80	195.0
128.00	149.0
134.80	111.0
140.90	336.0
142.90	577.0
156.90	110.0
172.00	224.0
174.00	23368.0
175.00	1932.0
176.00	22872.0
177.00	1446.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	501.0
37.00	2347.0
38.00	2051.0
39.00	879.0
39.90	252.0
44.00	836.0
44.90	404.0
47.00	503.0
48.00	308.0
49.00	1732.0
50.00	8508.0
51.00	2683.0
55.00	160.0
55.90	763.0
57.00	1280.0
59.90	429.0
61.00	2222.0
62.00	2252.0
63.00	1615.0
63.90	191.0
65.00	123.0
67.00	179.0
68.00	4133.0
69.00	4057.0
70.00	471.0
72.00	263.0
73.00	2059.0
74.00	7199.0
75.00	19288.0
76.00	1714.0
77.00	279.0
78.10	149.0
78.90	1866.0
79.90	491.0
80.90	1689.0
81.90	482.0
87.10	1618.0
87.90	1263.0
90.90	187.0
92.00	1071.0
93.00	1643.0
94.10	4738.0
95.10	34344.0
96.00	2537.0
104.00	155.0
105.90	227.0
115.90	176.0
116.90	291.0
117.90	160.0
118.80	236.0
127.90	149.0
129.00	103.0
130.00	111.0
134.80	159.0
140.90	395.0
142.90	629.0
157.00	120.0
172.00	235.0
174.00	25552.0
175.00	2067.0
176.00	24768.0
177.00	1648.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	463.0
37.00	2314.0
38.00	2168.0
39.10	893.0
39.90	276.0
44.10	905.0
45.00	439.0
47.00	471.0
47.90	253.0
49.00	1754.0
50.00	8326.0
51.00	2712.0
54.90	132.0
55.90	756.0
57.00	1149.0
59.90	378.0
61.00	2320.0
62.00	2056.0
63.00	1561.0
64.00	164.0
64.90	133.0
67.00	178.0
68.00	4098.0
69.00	4225.0
70.00	431.0
72.00	233.0
73.10	1873.0
74.00	7376.0
75.00	19248.0
76.00	1705.0
77.00	225.0
78.10	101.0
78.90	1823.0
79.90	458.0
80.90	1753.0
81.90	487.0
87.00	1543.0
88.00	1235.0
90.90	173.0
92.00	1023.0
93.00	1682.0
94.00	5100.0
95.10	33832.0
96.00	2206.0
103.80	217.0
104.80	105.0
106.00	246.0
115.90	177.0
116.90	257.0
117.90	162.0
118.80	247.0
127.80	134.0
129.00	105.0
129.90	157.0
134.80	153.0
140.90	451.0
142.90	568.0
157.00	103.0
172.00	222.0
174.00	25432.0
175.00	2089.0
176.00	24672.0
177.00	1625.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

Scan 2848 (10.248 min): VU034882.D
BFB40

m/z	Abundance
39.90	266.0
43.90	775.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40