
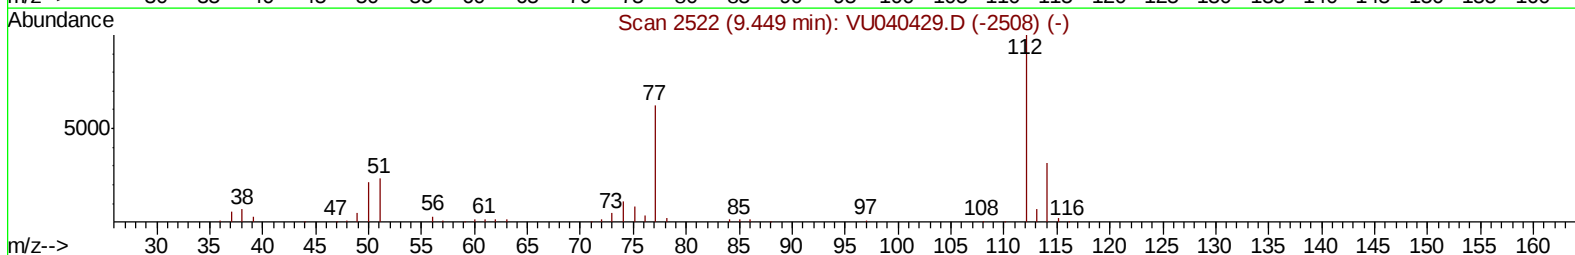
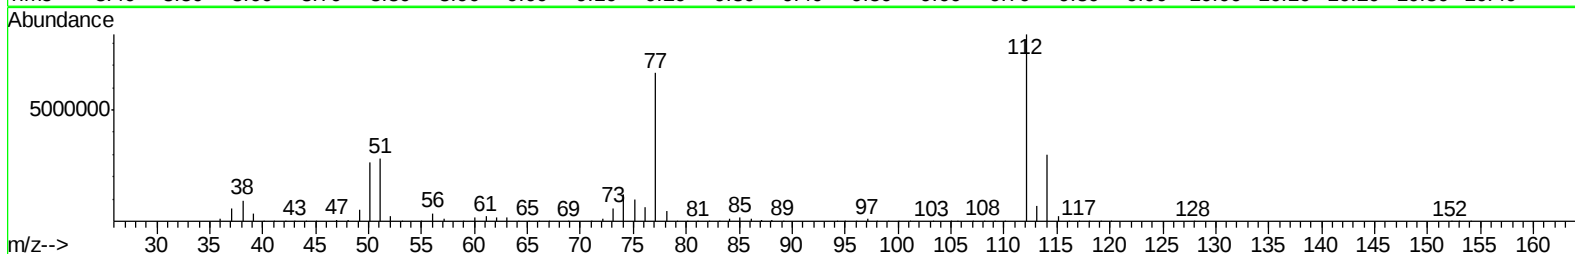


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100120\
 Data File : VU040437.D
 Acq On : 01 Oct 2020 22:14
 Operator : SY/MD
 Sample : L4240-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Quant Time: Oct 02 05:28:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 05:20:15 2020
 Response via : Initial Calibration

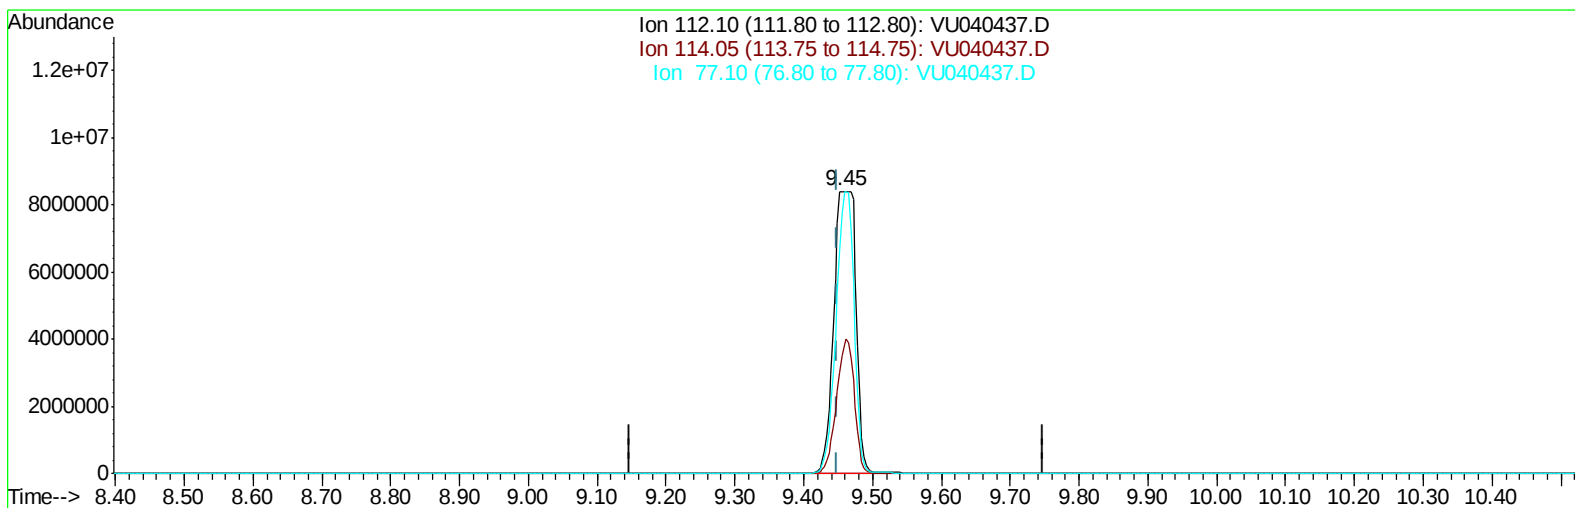

TIC: VU040437.D

(51) Chlorobenzene (T)

9.452min (+0.003) 650.98ug/L m

response 18793153

Ion	Exp%	Act%
112.10	100	100
114.05	31.40	35.77
77.10	61.90	79.23#
0.00	0.00	0.00