
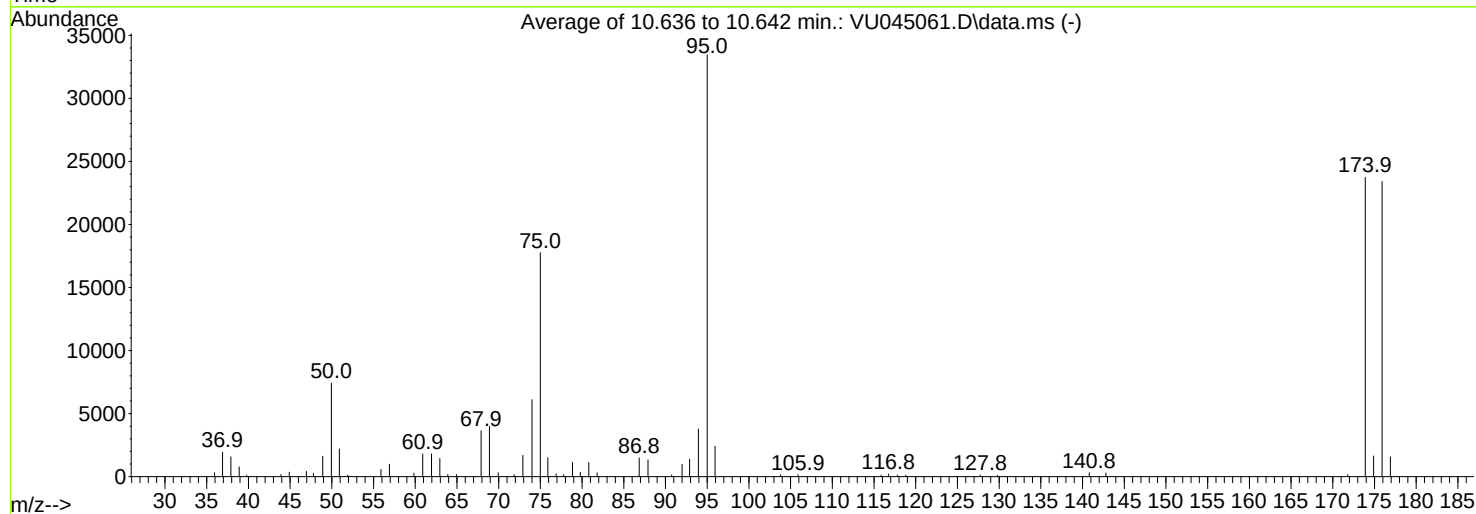


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100121\
Data File : VU045061.D
Acq On : 01 Oct 2021 08:58
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
Title : SW846 8260
Last Update : Tue Sep 28 12:32:13 2021

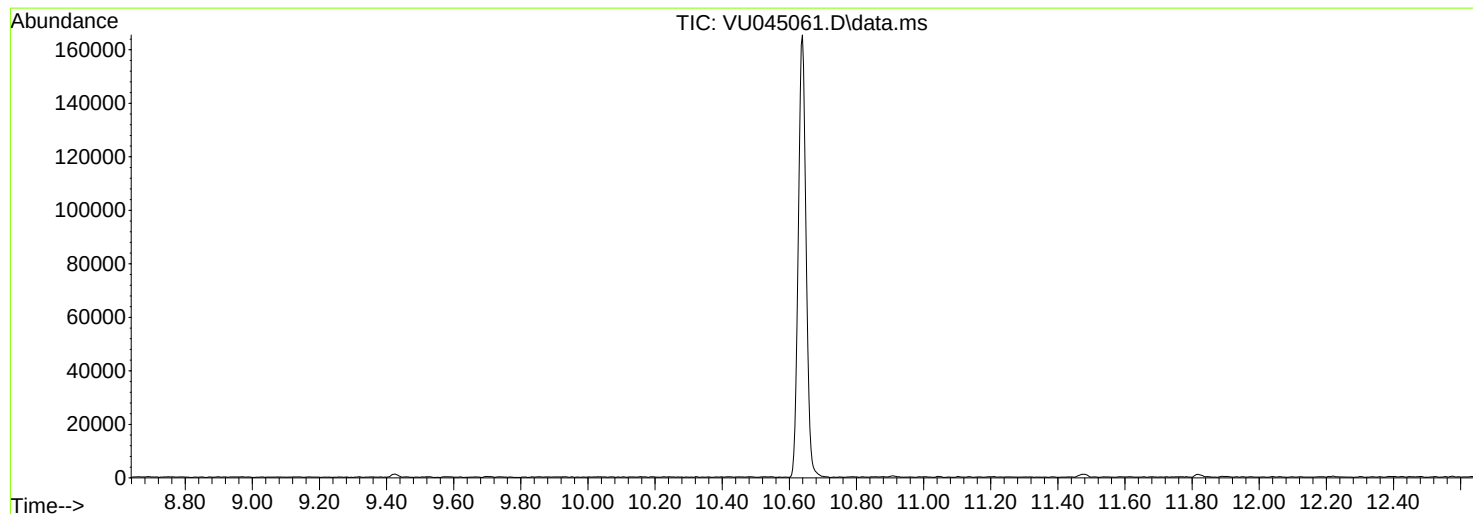

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.2	7413	PASS
75	95	30	60	53.1	17763	PASS
95	95	100	100	100.0	33451	PASS
96	95	5	9	7.2	2415	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.9	23731	PASS
175	174	5	9	6.9	1640	PASS
176	174	95	101	98.7	23411	PASS
177	176	5	9	6.7	1558	PASS