

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100124\
 Data File : VU061049.D
 Acq On : 01 Oct 2024 17:25
 Operator : MD/SY
 Sample : P4227-04 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-9D(20240926)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	109	rBV	85584	96545	7.10%	1.271%
2	1.911	186	193	206	rBV	62653	81178	5.97%	1.068%
3	2.563	385	396	415	rVB	134439	221459	16.30%	2.915%
4	3.177	577	587	603	rVB	13753	29678	2.18%	0.391%
5	4.631	1025	1039	1073	rBV2	105522	303238	22.32%	3.991%
6	5.055	1156	1171	1191	rBV	116537	262760	19.34%	3.458%
7	5.718	1358	1377	1405	rBV2	242600	634928	46.72%	8.356%
8	6.242	1528	1540	1572	rBV	222860	445463	32.78%	5.863%
9	6.682	1662	1677	1703	rBV	151055	304858	22.43%	4.012%
10	7.560	1938	1950	1975	rBV	81991	156635	11.53%	2.061%
11	7.891	2041	2053	2074	rBV	299584	541013	39.81%	7.120%
12	8.174	2129	2141	2166	rBV	49336	94446	6.95%	1.243%
13	8.627	2271	2282	2324	rBV	345531	701157	51.60%	9.228%
14	9.412	2514	2526	2554	rBV	313110	615688	45.31%	8.103%
15	10.746	2931	2941	2956	rBV	102106	169318	12.46%	2.228%
16	11.740	3239	3250	3260	rBV	76994	124239	9.14%	1.635%
17	11.807	3260	3271	3303	rVB2	341234	919872	67.69%	12.106%
18	12.187	3375	3389	3412	rBV	264163	479536	35.29%	6.311%
19	13.833	3888	3901	3923	rBV	829443	1358863	100.00%	17.883%
20	14.325	4041	4054	4068	rBV2	32425	57582	4.24%	0.758%

Sum of corrected areas: 7598456




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100124\
Data File : VU061049.D
Acq On : 01 Oct 2024 17:25
Operator : MD/SY
Sample : P4227-04 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-9D(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

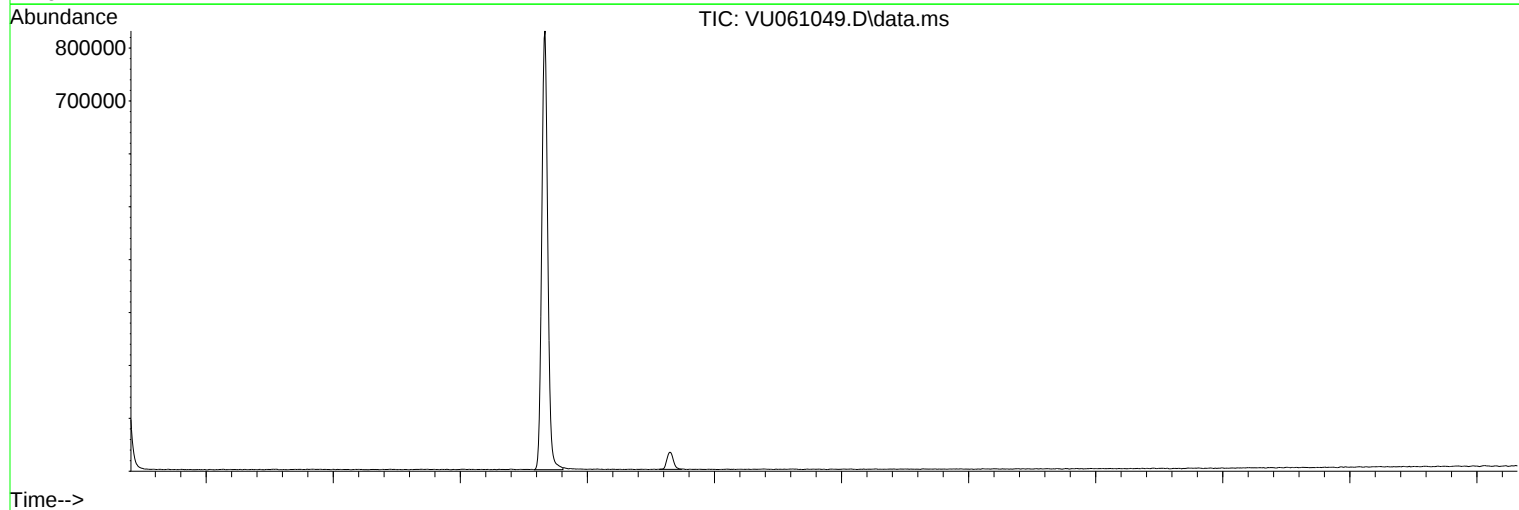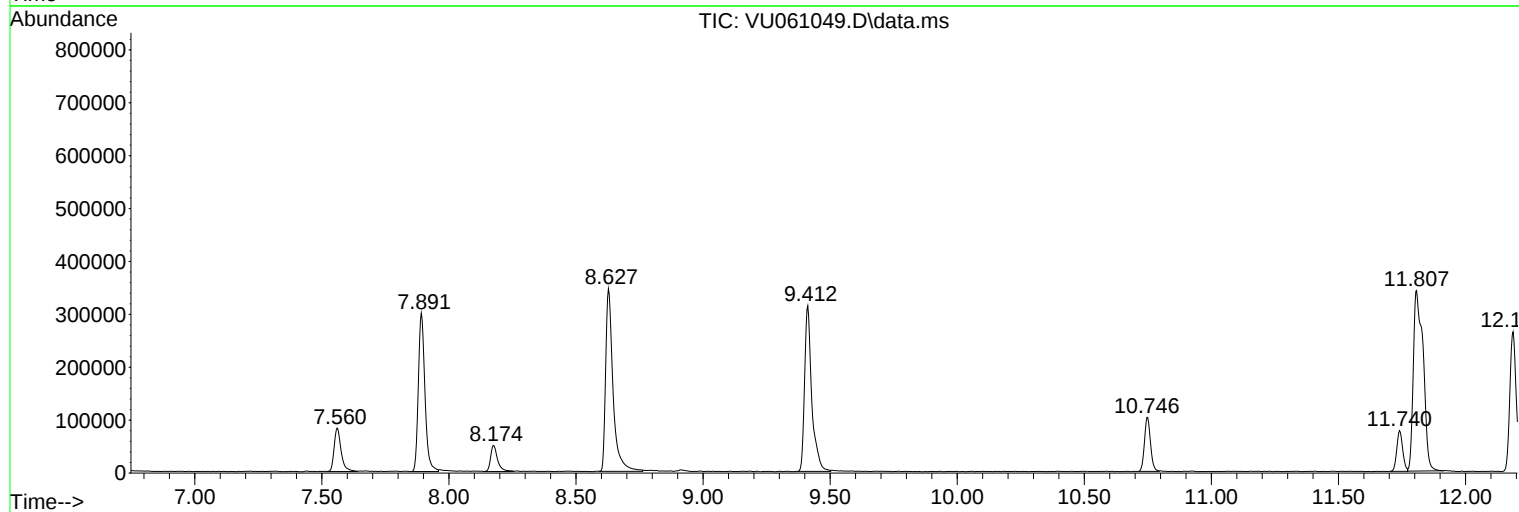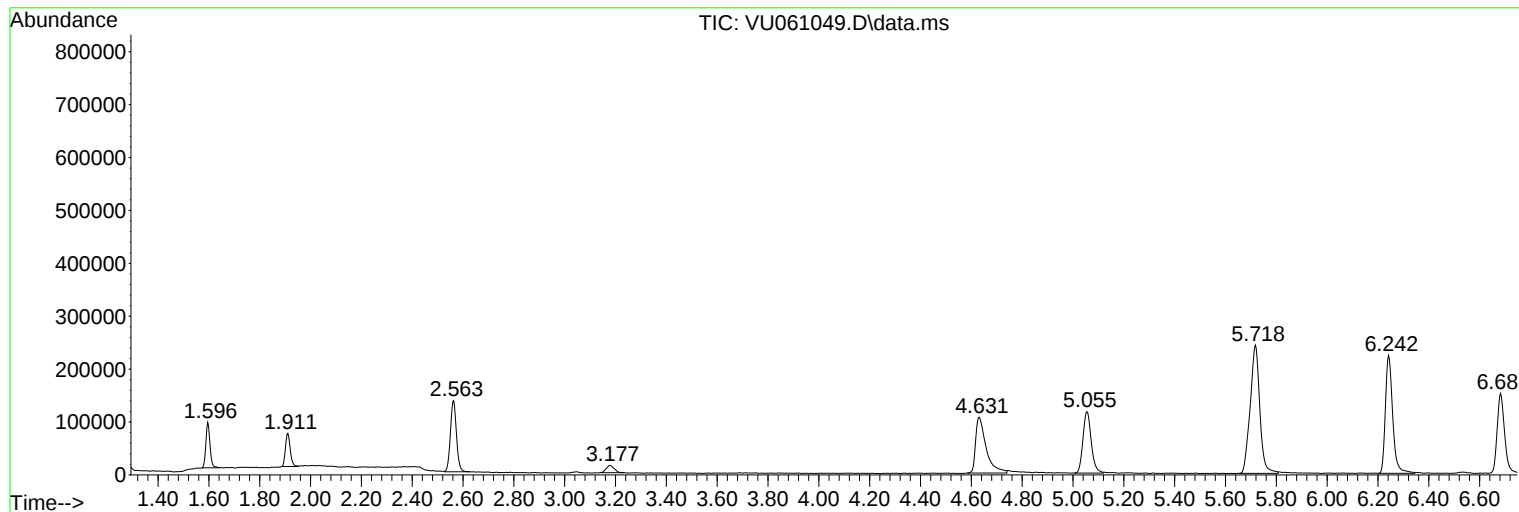

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100124\
Data File : VU061049.D
Acq On : 01 Oct 2024 17:25
Operator : MD/SY
Sample : P4227-04 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-9D(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100124\
Data File : VU061049.D
Acq On : 01 Oct 2024 17:25
Operator : MD/SY
Sample : P4227-04 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-9D(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------