

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100124\
 Data File : VU061060.D
 Acq On : 01 Oct 2024 21:53
 Operator : MD/SY
 Sample : P4227-07 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DUP(20240926)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	107	rBV	79445	89165	11.62%	1.588%
2	1.911	185	193	203	rBV	60496	77986	10.16%	1.389%
3	2.563	383	396	414	rBV	120543	197127	25.69%	3.511%
4	3.174	575	586	603	rVB2	6785	16392	2.14%	0.292%
5	4.634	1024	1040	1081	rBV2	99326	308473	40.20%	5.494%
6	5.055	1157	1171	1193	rBV	106635	238783	31.12%	4.253%
7	5.718	1356	1377	1414	rBV2	216747	587181	76.52%	10.458%
8	6.242	1528	1540	1567	rBV	212989	429725	56.00%	7.654%
9	6.682	1662	1677	1700	rBV	140273	286319	37.31%	5.100%
10	7.560	1939	1950	1972	rBV2	73506	140813	18.35%	2.508%
11	7.891	2040	2053	2074	rBV	267915	488622	63.67%	8.703%
12	8.177	2130	2142	2162	rBV	43462	83909	10.93%	1.495%
13	8.631	2272	2283	2316	rBV	309163	658701	85.84%	11.732%
14	9.412	2511	2526	2559	rBV2	300418	767389	100.00%	13.668%
15	10.746	2925	2941	2956	rBV	94314	160491	20.91%	2.859%
16	11.740	3240	3250	3260	rBV	97632	161487	21.04%	2.876%
17	11.807	3260	3271	3274	rBV	325728	499952	65.15%	8.905%
18	12.187	3376	3389	3407	rBV	230067	409128	53.31%	7.287%
19	13.849	3896	3906	3915	rBV4	6911	12773	1.66%	0.228%

Sum of corrected areas: 5614416




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100124\
Data File : VU061060.D
Acq On : 01 Oct 2024 21:53
Operator : MD/SY
Sample : P4227-07 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

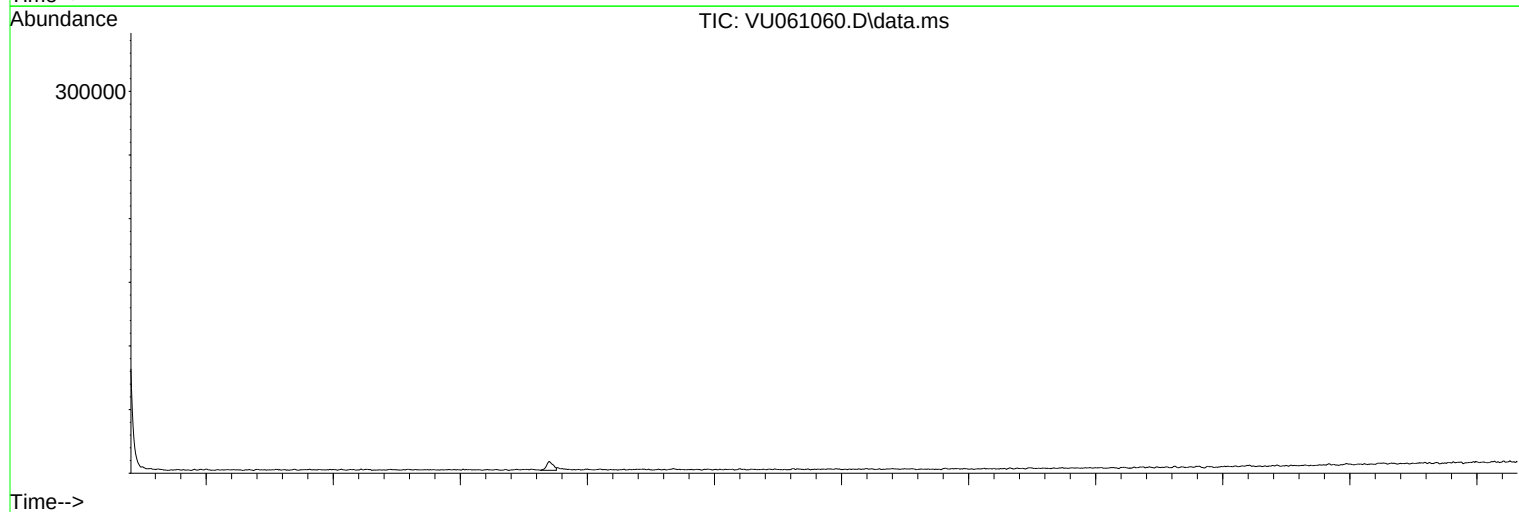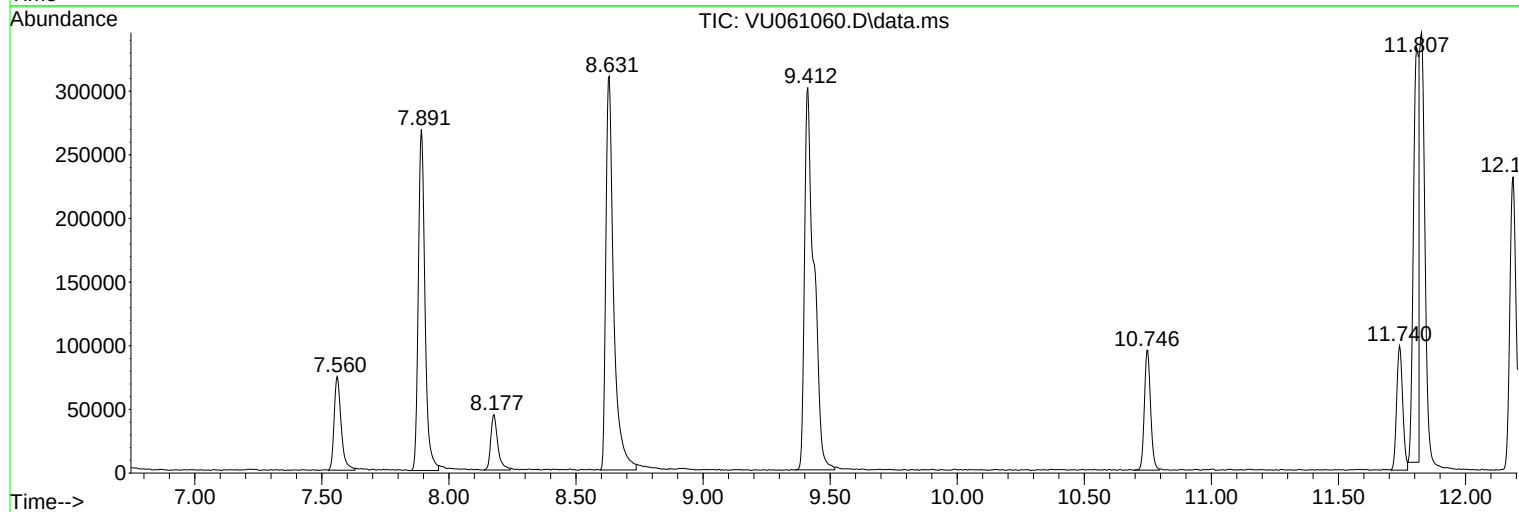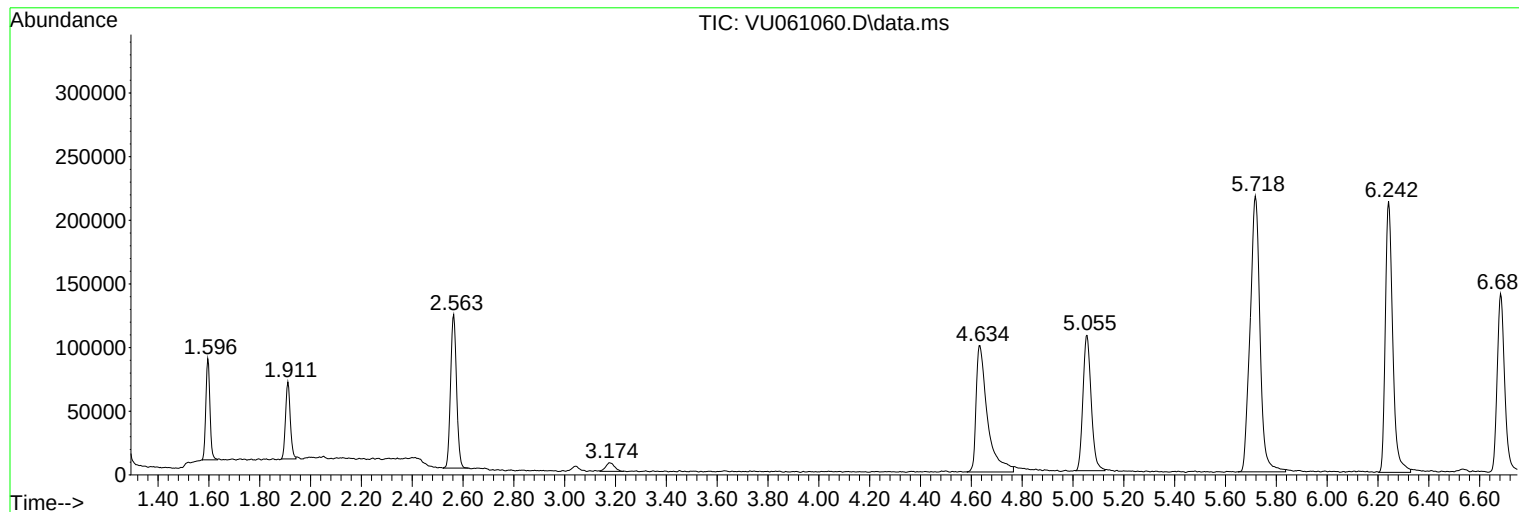

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100124\
Data File : VU061060.D
Acq On : 01 Oct 2024 21:53
Operator : MD/SY
Sample : P4227-07 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100124\
Data File : VU061060.D
Acq On : 01 Oct 2024 21:53
Operator : MD/SY
Sample : P4227-07 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------