
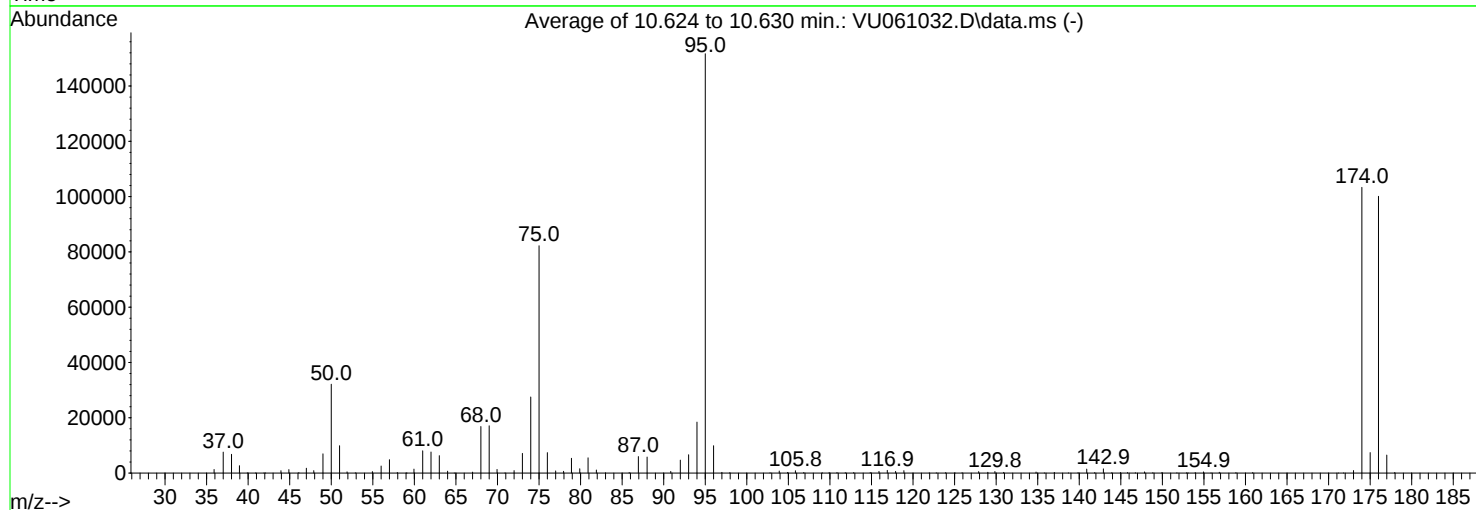


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100124\
Data File : VU061032.D
Acq On : 01 Oct 2024 08:55
Operator : MD/SY
Sample : BFB008
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB008

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Oct 02 02:09:38 2024

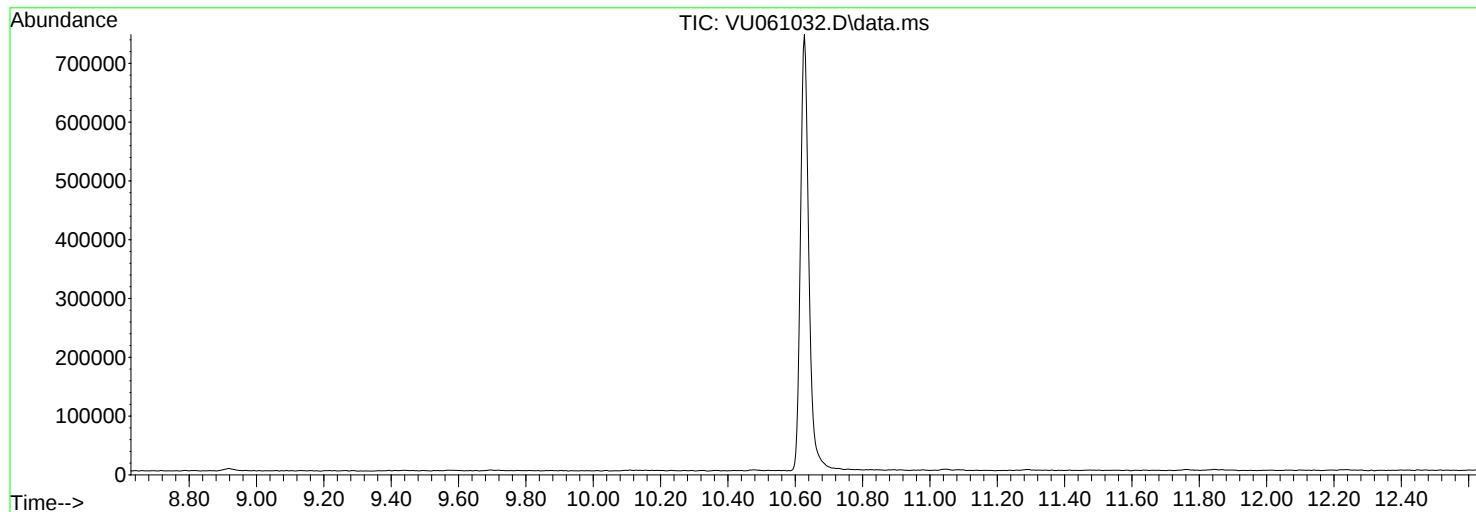

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2887

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	32131	PASS
75	95	30	80	54.2	82235	PASS
95	95	100	100	100.0	151676	PASS
96	95	5	9	6.5	9908	PASS
173	174	0.00	2	0.9	930	PASS
174	95	50	120	68.1	103331	PASS
175	174	5	9	7.2	7423	PASS
176	174	95	101	96.9	100112	PASS
177	176	5	9	6.5	6516	PASS

m/z	Abundance
36.00	158.0
38.00	129.0
39.00	269.0
39.90	193.0
41.00	398.0
42.00	138.0
42.90	477.0
44.00	1298.0
44.90	102.0
53.90	148.0
54.90	302.0
56.00	247.0
57.00	294.0
58.00	203.0
59.00	159.0
67.00	183.0
68.00	107.0
69.00	247.0
69.90	135.0
70.90	214.0
77.00	106.0
79.00	153.0
81.10	125.0
81.90	146.0
83.00	198.0
83.90	125.0
85.00	113.0
90.80	127.0
95.00	132.0
96.00	175.0
97.00	149.0
239.20	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
35.90	1406.0
37.00	7653.0
38.00	7077.0
39.00	2956.0
39.90	294.0
40.90	446.0
41.90	154.0
42.10	153.0
43.00	453.0
43.90	2159.0
45.00	1397.0
46.10	176.0
47.00	1772.0
47.90	899.0
49.00	6812.0
50.00	32528.0
51.00	10074.0
51.90	425.0
52.90	116.0
54.10	122.0
55.00	834.0
56.00	2837.0
57.00	5152.0
58.00	402.0
59.00	181.0
59.90	1409.0
61.00	8227.0
62.00	7588.0
63.00	6282.0
64.00	715.0
67.00	549.0
68.00	17016.0
69.00	17576.0
70.00	1475.0
70.90	278.0
72.00	823.0
73.00	7134.0
74.00	27304.0
75.00	82928.0
76.00	7760.0
77.00	878.0
77.90	620.0
78.90	5560.0
79.90	1582.0
80.90	5722.0
81.90	1241.0
83.00	314.0
84.00	103.0
85.90	218.0
87.00	5923.0
88.00	5527.0
90.90	777.0
92.00	4686.0
93.00	6665.0
94.00	18512.0
95.00	152128.0
96.00	10238.0
97.00	395.0
98.00	122.0
102.80	122.0
103.90	703.0
104.90	249.0
105.80	843.0
106.90	241.0
109.10	151.0
109.90	162.0
110.80	221.0
112.00	155.0
112.80	172.0
114.90	221.0
115.90	592.0
116.90	1078.0
117.90	624.0
118.90	866.0
122.80	103.0
123.90	153.0
125.00	105.0
125.90	136.0
127.90	529.0
129.00	297.0
129.90	586.0
130.90	265.0
134.80	368.0
135.80	115.0
137.00	259.0
139.90	149.0
140.90	1465.0
141.90	180.0
142.90	1493.0
143.90	115.0
144.90	188.0
145.80	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

146.70	138.0
147.80	438.0
148.80	138.0
150.00	224.0
151.70	111.0
152.90	158.0
153.90	137.0
155.00	376.0
156.80	259.0
158.90	201.0
160.90	182.0
171.20	116.0
171.80	151.0
173.00	904.0
174.00	100496.0
175.00	7317.0
176.00	98008.0
177.00	6388.0
178.00	185.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
35.90	1507.0
37.00	7848.0
38.00	7136.0
39.00	3031.0
39.90	289.0
40.90	466.0
41.90	173.0
43.00	428.0
44.00	2195.0
45.00	1415.0
46.10	193.0
47.00	1813.0
47.90	908.0
49.00	7153.0
50.00	33128.0
51.00	10169.0
51.90	468.0
52.90	117.0
54.10	109.0
55.00	860.0
56.00	2864.0
57.00	5344.0
58.00	434.0
59.10	159.0
60.00	1513.0
61.00	8339.0
62.00	7883.0
63.00	6525.0
64.00	720.0
67.00	544.0
68.00	17480.0
69.00	17864.0
70.00	1485.0
70.90	279.0
72.00	932.0
73.00	7342.0
74.00	28352.0
75.00	84704.0
76.00	7623.0
77.00	912.0
78.00	661.0
78.90	5663.0
79.90	1583.0
80.90	5841.0
81.90	1295.0
83.00	277.0
84.00	114.0
85.10	116.0
85.80	224.0
86.90	6114.0
88.00	5987.0
90.90	750.0
92.00	4815.0
93.00	6822.0
94.00	19048.0
95.00	156352.0
96.00	10336.0
97.00	429.0
97.90	141.0
102.80	141.0
103.90	768.0
104.90	244.0
105.90	869.0
106.80	231.0
109.10	127.0
109.90	178.0
110.90	220.0
111.80	151.0
112.80	177.0
114.80	215.0
115.90	611.0
116.90	1010.0
117.90	620.0
118.90	930.0
121.90	109.0
122.80	108.0
123.90	139.0
125.10	105.0
125.90	133.0
127.90	575.0
129.00	313.0
129.90	567.0
130.90	271.0
134.80	400.0
135.80	113.0
137.00	239.0
138.70	107.0
139.80	162.0
140.90	1492.0
141.80	181.0
142.90	1581.0
143.90	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

144.90	173.0
145.80	212.0
146.70	133.0
147.90	468.0
148.80	144.0
150.00	219.0
151.80	125.0
152.90	158.0
154.00	160.0
154.90	455.0
155.80	102.0
156.90	303.0
158.80	190.0
160.80	179.0
173.00	956.0
174.00	106696.0
175.00	7644.0
176.00	103128.0
177.00	6698.0
178.00	190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
35.90	1467.0
37.00	7294.0
38.00	6538.0
38.90	2867.0
39.90	294.0
40.90	469.0
41.90	182.0
43.00	450.0
44.00	2161.0
44.90	1310.0
46.10	196.0
47.00	1695.0
47.90	858.0
49.00	6957.0
50.00	30736.0
51.00	9451.0
51.90	462.0
52.90	112.0
55.00	821.0
56.00	2682.0
57.00	4937.0
57.90	416.0
59.10	150.0
60.00	1418.0
61.00	7620.0
62.00	7378.0
63.00	6086.0
64.00	643.0
64.80	111.0
67.00	513.0
68.00	16347.0
69.00	16632.0
70.00	1442.0
70.90	254.0
72.00	945.0
73.00	6864.0
74.00	26880.0
75.00	79072.0
76.00	6830.0
77.00	884.0
78.00	652.0
78.90	5295.0
79.90	1516.0
80.90	5413.0
81.90	1242.0
83.00	253.0
84.00	126.0
85.00	149.0
85.80	192.0
86.90	5893.0
88.00	5877.0
90.90	673.0
92.00	4546.0
93.00	6436.0
94.00	17768.0
95.00	146944.0
96.00	9675.0
97.00	434.0
98.00	148.0
102.80	136.0
103.90	769.0
104.90	242.0
105.90	838.0
106.80	213.0
109.90	185.0
110.90	233.0
111.80	152.0
112.90	181.0
114.80	212.0
115.90	626.0
116.90	889.0
117.90	597.0
118.90	889.0
122.00	113.0
122.80	100.0
123.90	127.0
125.90	116.0
127.90	534.0
129.00	311.0
129.80	559.0
130.90	269.0
134.80	372.0
137.00	243.0
138.70	104.0
139.80	155.0
140.90	1362.0
141.80	180.0
142.90	1506.0
143.90	118.0
145.00	161.0
145.80	218.0
146.80	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

147.90	429.0
148.90	140.0
149.90	190.0
151.80	131.0
153.10	147.0
154.00	172.0
154.90	485.0
155.90	113.0
156.90	314.0
158.80	188.0
160.80	189.0
173.00	930.0
174.00	102800.0
175.00	7309.0
176.00	99200.0
177.00	6462.0
177.90	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008