
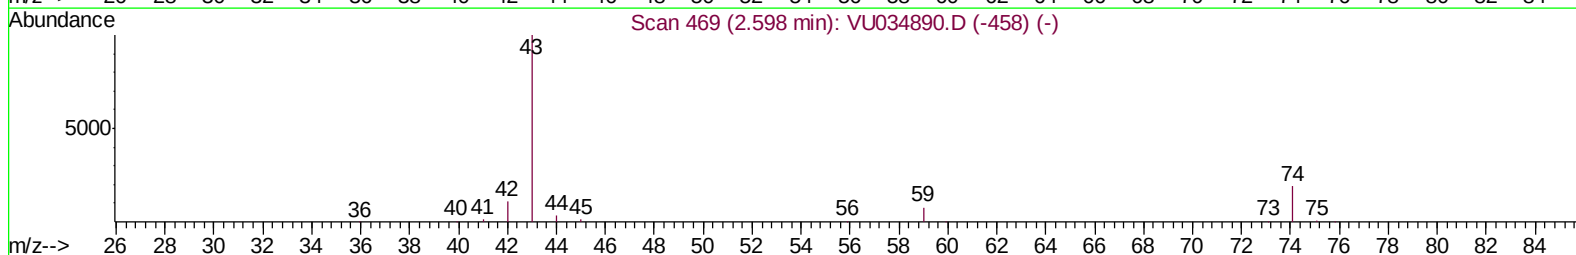
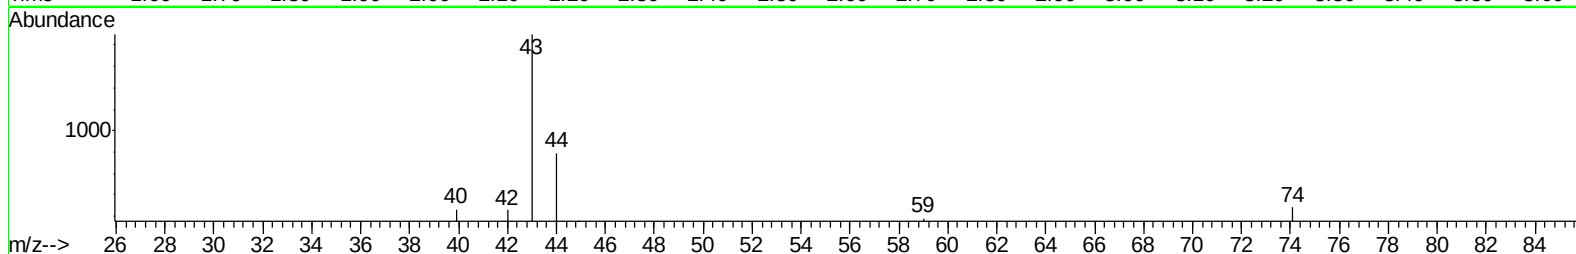


Data File : VU034898.D
Acq On : 01 Oct 2019 19:20
Operator : JC/SP
Sample : K5028-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Oct 02 01:54:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 02 01:50:17 2019
Response via : Initial Calibration

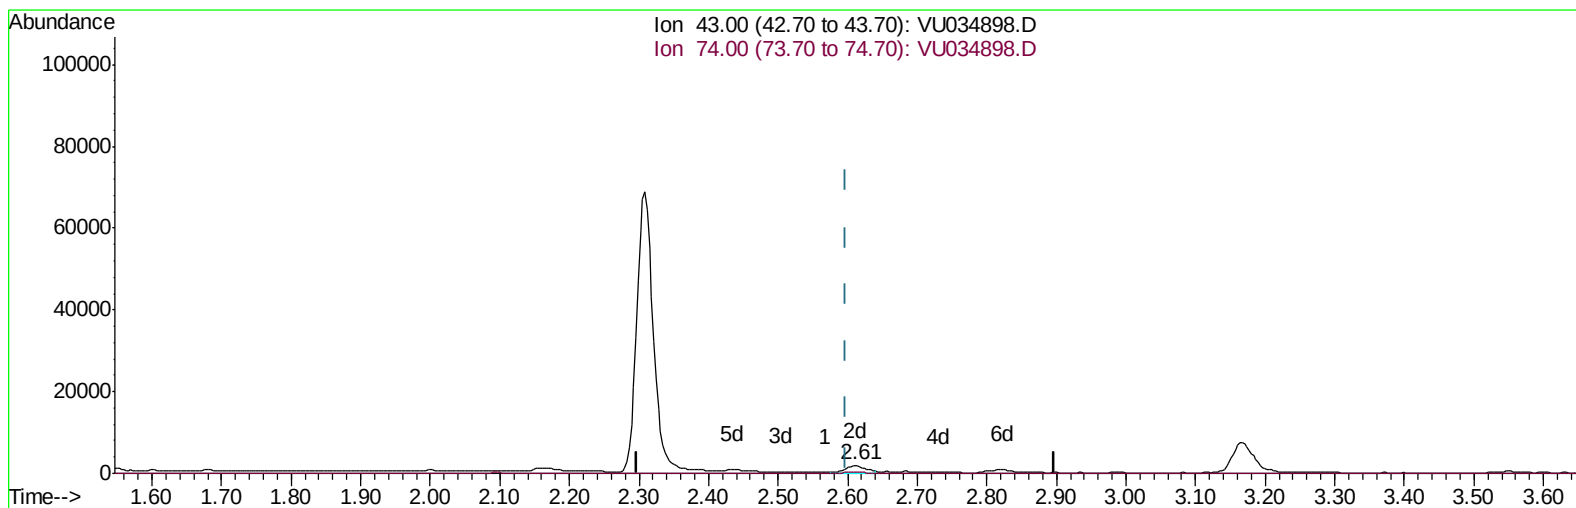

TIC: VU034898.D

(15) Methyl Acetate (T)

2.611min (+0.013) 1.40ug/L m

response 4279

Ion	Exp%	Act%
43.00	100	100
74.00	19.10	4.95#
0.00	0.00	0.00
0.00	0.00	0.00