
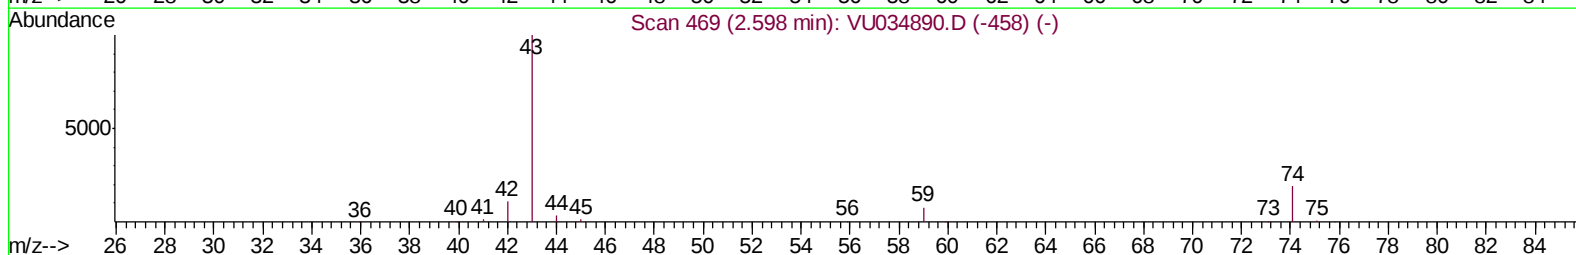
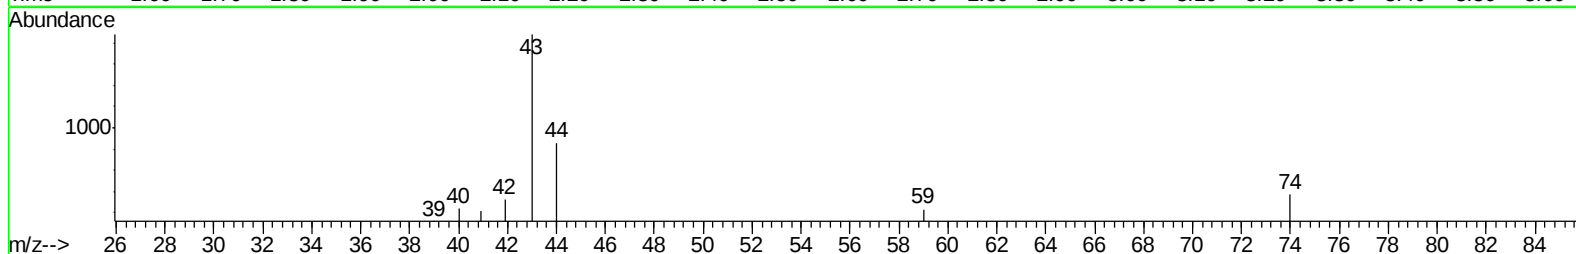


Data File : VU034906.D
Acq On : 01 Oct 2019 22:28
Operator : JC/SP
Sample : K5028-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Oct 02 01:57:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 02 01:50:17 2019
Response via : Initial Calibration

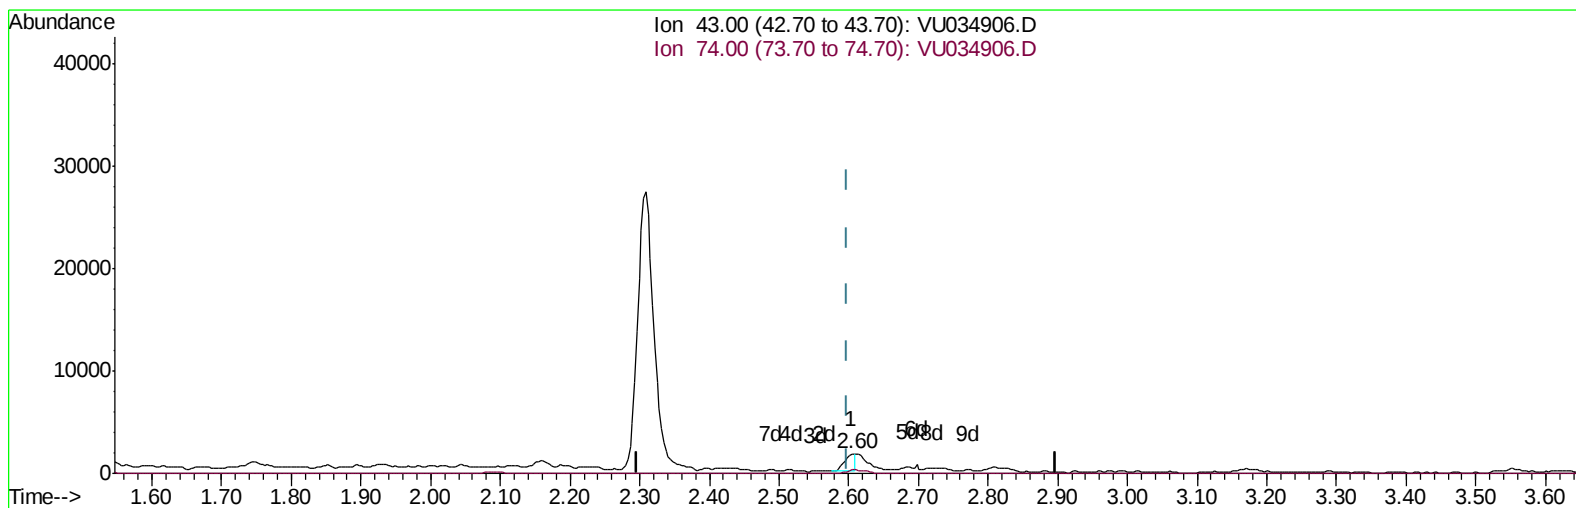

TIC: VU034906.D

(15) Methyl Acetate (T)

2.605min (+0.007) 0.53ug/L

response 1615

Ion	Exp%	Act%
43.00	100	100
74.00	19.10	42.60#
0.00	0.00	0.00
0.00	0.00	0.00