


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU100219\
Quantitation Report (QT/LSC Reviewed)
Data File : VU034904.D
Acq On : 01 Oct 2019 21:41
Operator : JC/SP
Sample : K5028-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDL8

Manual Integrations
APPROVED

MMDadoda
10/4/2019 12:14:09 PM

Quant Time: Oct 02 04:36:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 02 01:50:17 2019
Response via : Initial Calibration

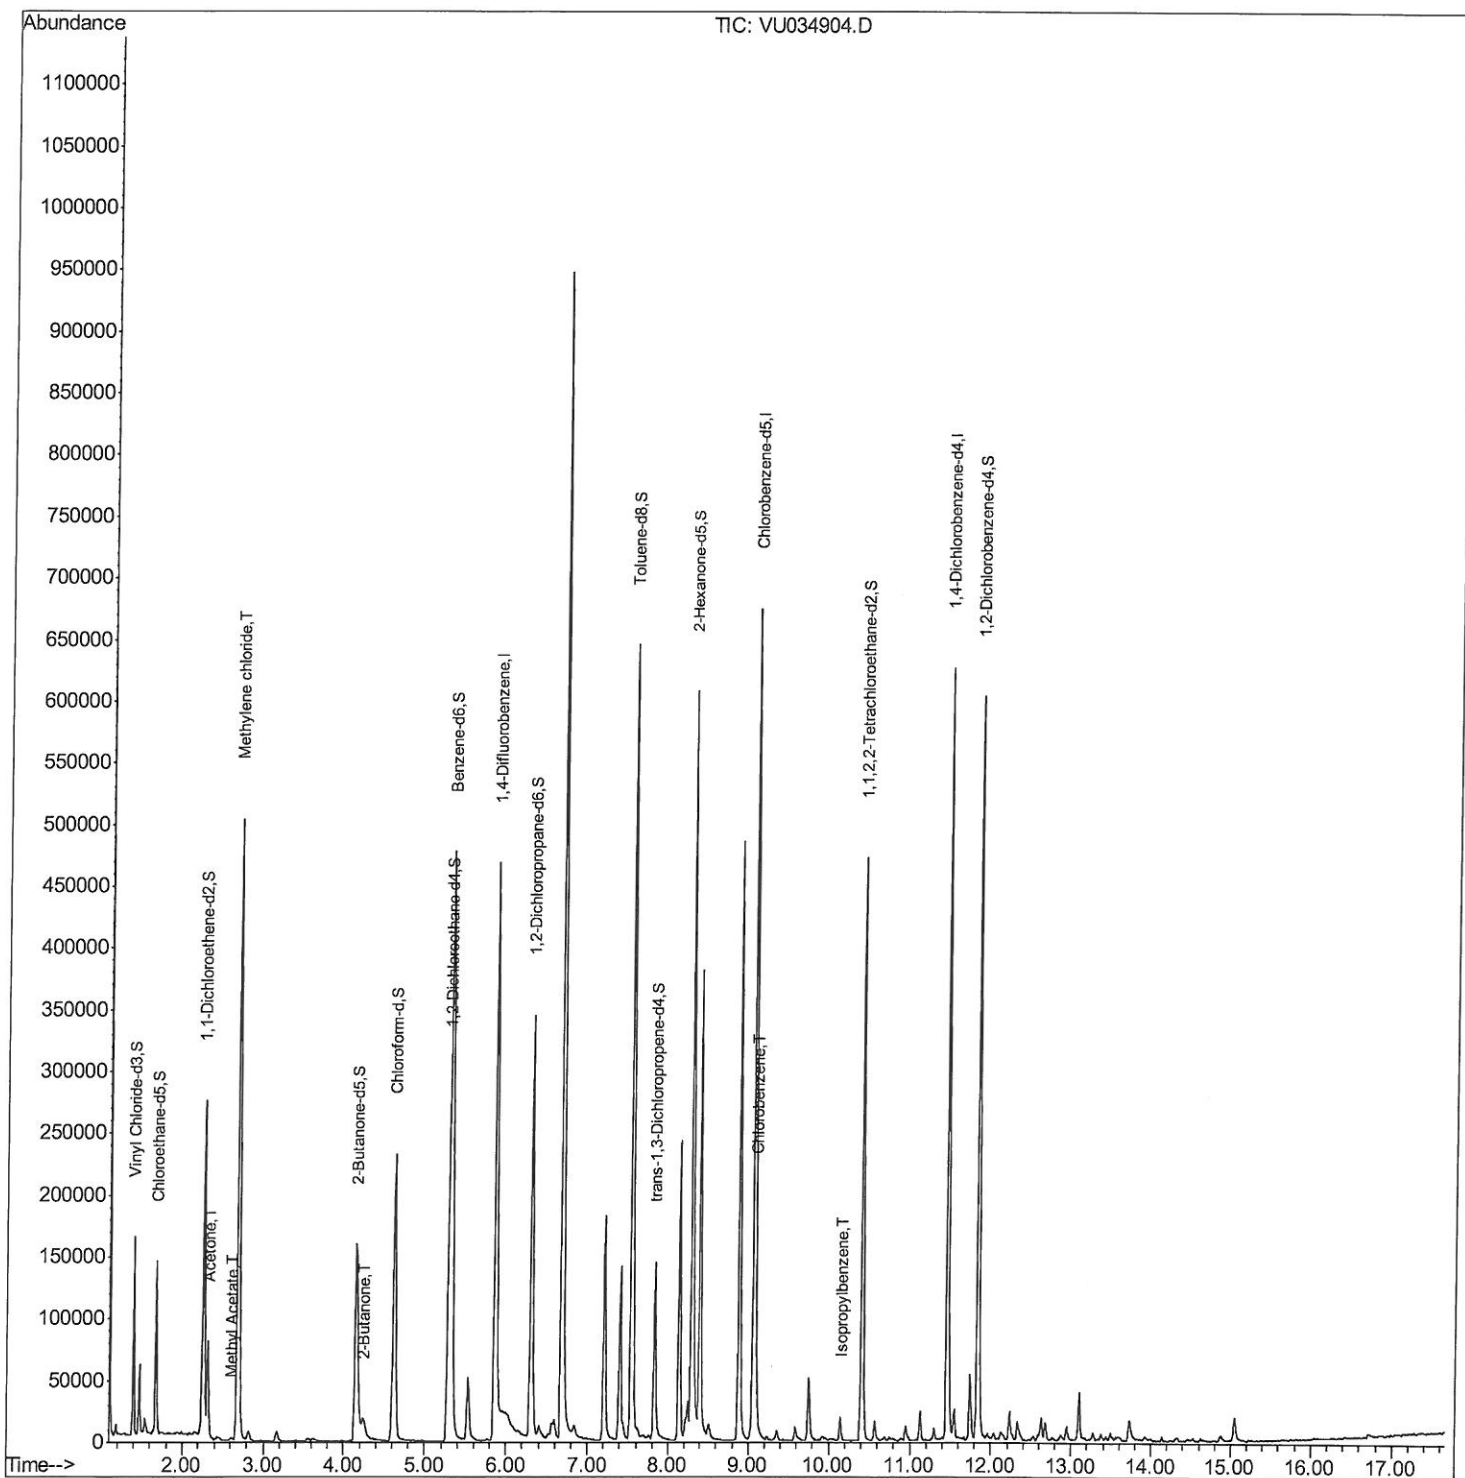

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU100219\
Quantitation Report (Qedit)




Data File : VU034904.D
Acq On : 01 Oct 2019 21:41
Operator : JC/SP
Sample : K5028-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDL8

Manual Integrations
APPROVED

MMDadoda
10/4/2019 12:14:09 PM

Quant Time: Oct 02 01:56:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 02 01:50:17 2019
Response via : Initial Calibration

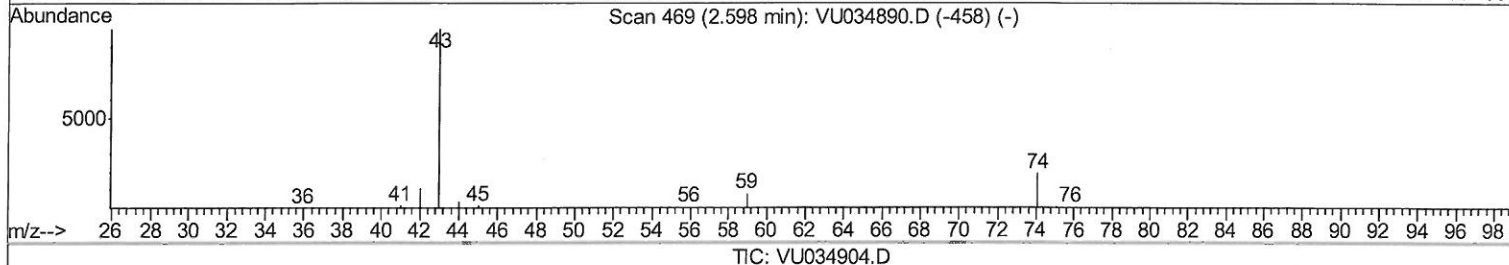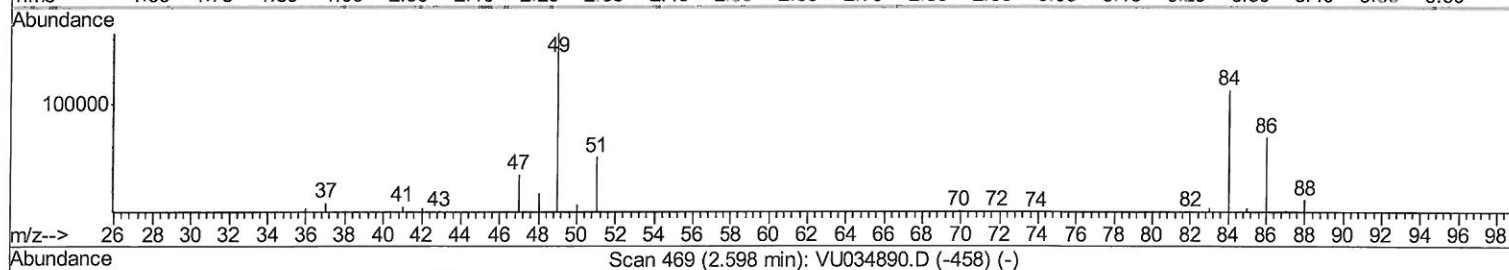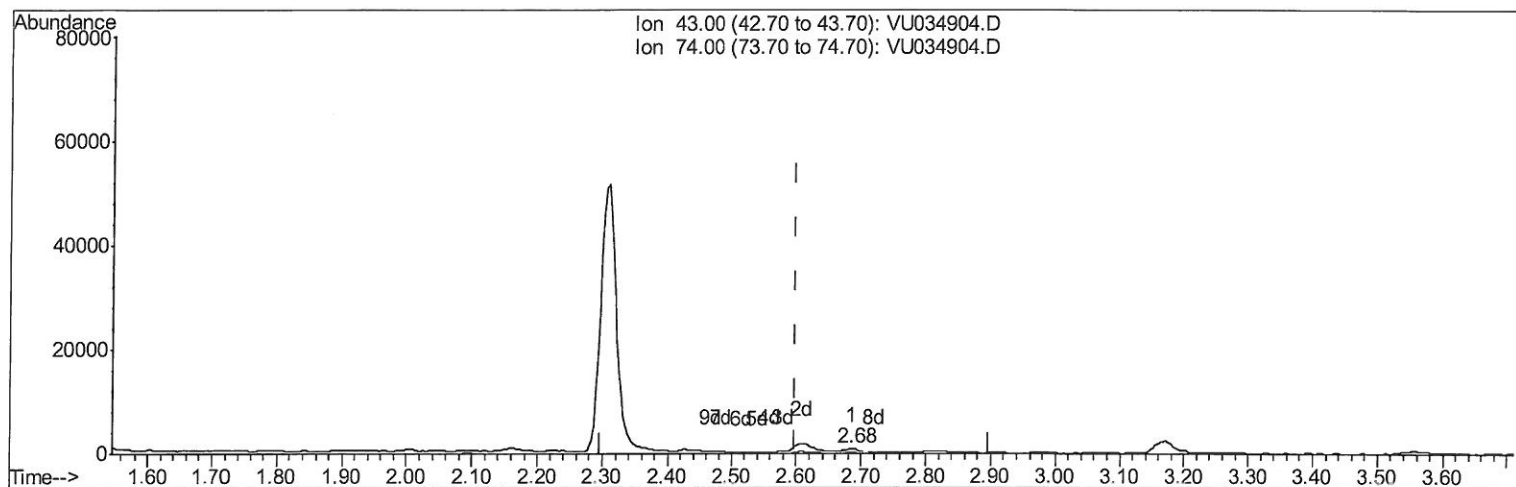

(15) Methyl Acetate (T)

2.685min (+0.087) 0.35ug/L

response 1081

Ion	Exp%	Act%
43.00	100	100
74.00	19.10	16.47
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU100219\
Quantitation Report (Qedit)




Data File : VU034904.D
Acq On : 01 Oct 2019 21:41
Operator : JC/SP
Sample : K5028-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDL8

Manual Integrations
APPROVED

MMDadoda
10/4/2019 12:14:09 PM

Quant Time: Oct 02 01:56:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 02 01:50:17 2019
Response via : Initial Calibration

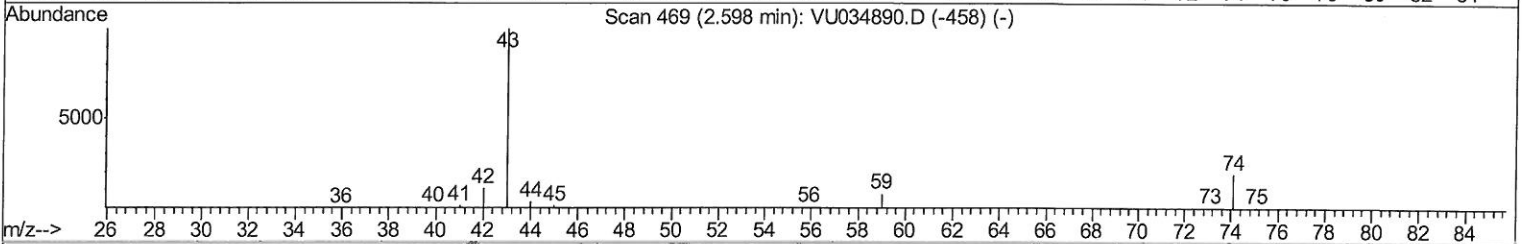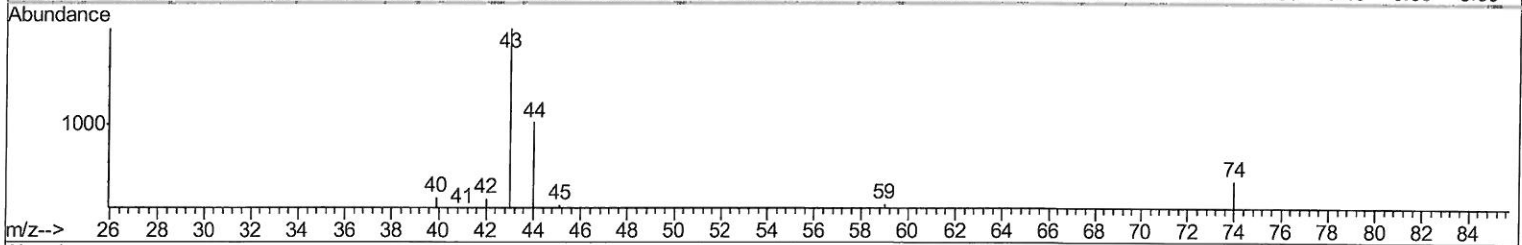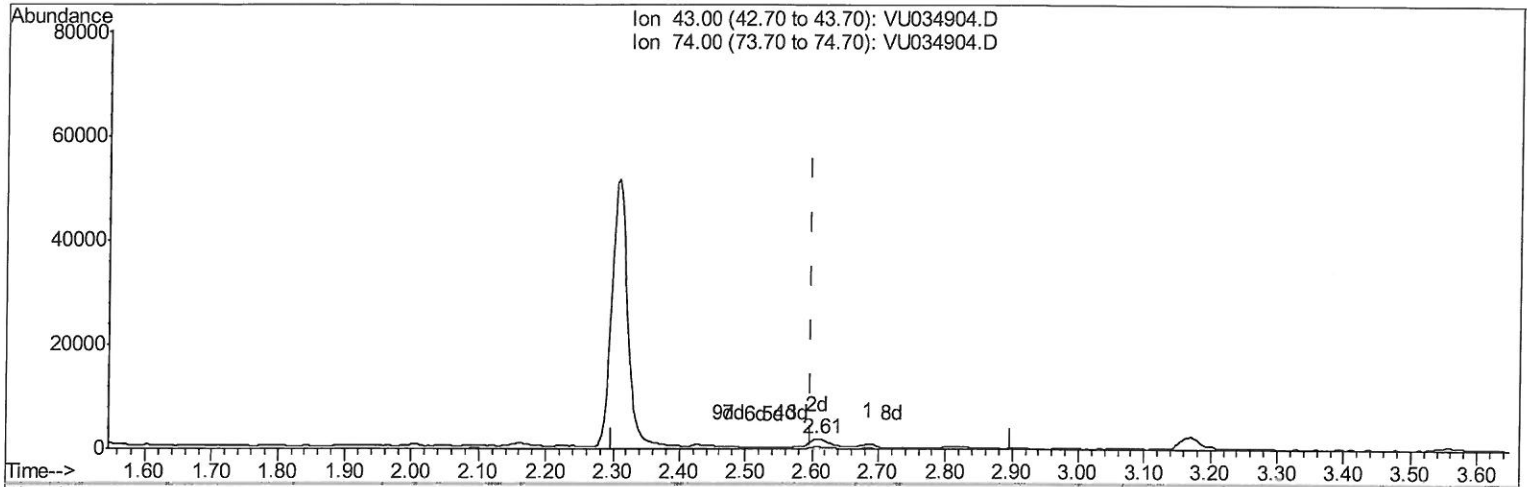

TIC: VU034904.D

(15) Methyl Acetate (T)

2.608min (+0.010) 1.32ug/L m

MO
10/04/19

response 4098

Ion	Exp%	Act%
43.00	100	100
74.00	19.10	4.34#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU100219\
 Quantitation Report (QT/LSC Reviewed)
 Data File : VU034904.D
 Acq On : 01 Oct 2019 21:41
 Operator : JC/SP
 Sample : K5028-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 BFDL8

Manual Integrations
 APPROVED

MMDadoda
 10/4/2019 12:14:09 PM

Quant Time: Oct 02 04:36:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 02 01:50:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.86	114	356853	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	347231	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.46	152	148236	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	99542	39.80	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.60%
7) Chloroethane-d5	1.67	69	90888	43.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.50%
11) 1,1-Dichloroethene-d2	2.26	63	152830	34.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.56%
21) 2-Butanone-d5	4.15	46	277563	113.73	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.73%
24) Chloroform-d	4.62	84	223604	46.07	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.14%
26) 1,2-Dichloroethane-d4	5.29	65	166111	46.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.22%
32) Benzene-d6	5.32	84	438903	46.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.88%
36) 1,2-Dichloropropane-d6	6.31	67	157531	48.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.94%
41) Toluene-d8	7.54	98	408035	45.88	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.76%
43) trans-1,3-Dichloropropene-	7.83	79	69216	48.09	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.18%
47) 2-Hexanone-d5	8.29	63	187417	120.48	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	120.48%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	222678	47.97	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.94%
64) 1,2-Dichlorobenzene-d4	11.84	152	146203	49.57	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.14%

Target Compounds

						Qvalue
13) Acetone	2.31	43	85104	43.875	ug/L	97
15) Methyl Acetate	2.61	43	4098m	1.324	ug/L	97
16) Methylene chloride	2.68	84	202892	103.784	ug/L	97
22) 2-Butanone	4.25	43	28087	11.149	ug/L	100
51) Chlorobenzene	9.10	112	15019	2.781	ug/L	95
56) Isopropylbenzene	10.14	105	12539	1.302	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MO
 10/04/19