


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100219\
Data File : VU034889.D
Acq On : 01 Oct 2019 14:48
Operator : JC/SP
Sample : BFB41
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100119WMA.M
Title : VOC Analysis
Last Update : Wed Oct 02 01:50:17 2019

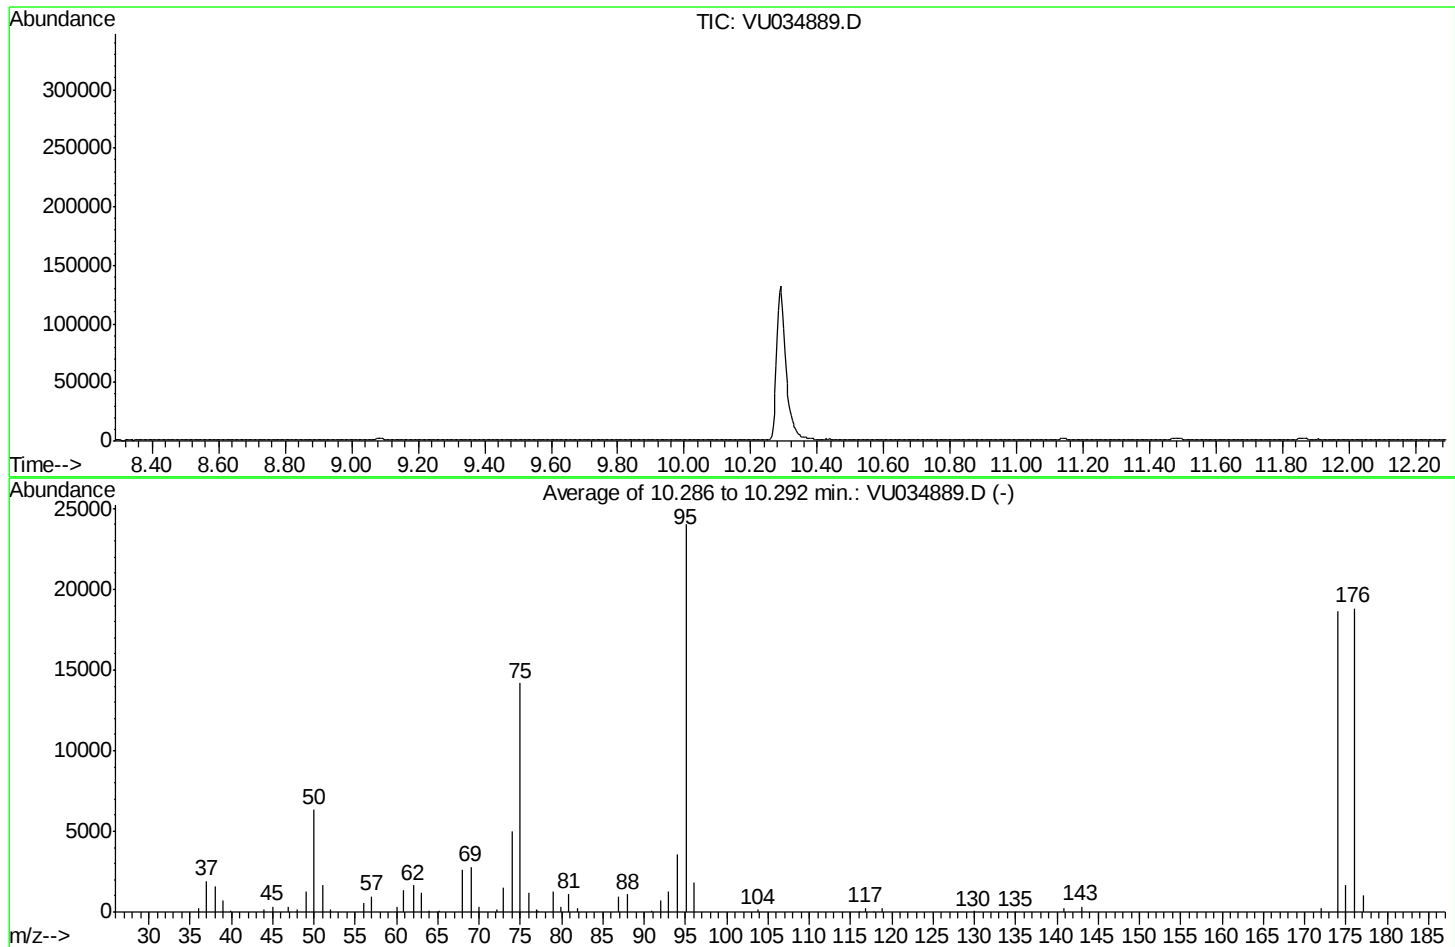

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.3	6330	PASS
75	95	30	80	59.1	14196	PASS
95	95	100	100	100.0	24026	PASS
96	95	5	9	7.7	1845	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.7	18666	PASS
175	174	5	9	8.8	1645	PASS
176	174	95	101	100.7	18805	PASS
177	176	5	9	5.6	1052	PASS

m/z	Abundance
36.00	289.0
37.00	2015.0
38.00	1485.0
39.00	689.0
40.00	306.0
43.90	936.0
45.00	362.0
46.90	325.0
47.90	201.0
49.00	1328.0
50.00	6030.0
51.00	1555.0
52.00	172.0
56.10	574.0
57.00	952.0
60.00	304.0
60.90	1363.0
62.00	1659.0
63.00	1276.0
64.90	126.0
68.00	2597.0
69.00	2681.0
70.00	309.0
72.10	174.0
73.00	1426.0
74.00	4920.0
75.00	14140.0
76.00	1284.0
76.90	202.0
78.90	1282.0
80.10	281.0
80.90	1168.0
81.90	261.0
86.90	862.0
88.00	1131.0
90.90	126.0
92.00	744.0
93.00	1107.0
94.00	3537.0
95.10	24104.0
96.00	1824.0
103.80	147.0
116.00	100.0
116.90	268.0
118.90	208.0
140.90	217.0
142.90	305.0
171.90	182.0
174.00	18520.0
175.00	1594.0
176.00	17888.0
177.10	1150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	245.0
37.00	2003.0
38.00	1607.0
38.90	711.0
40.00	272.0
43.90	957.0
45.00	370.0
46.90	384.0
47.90	201.0
49.00	1381.0
50.00	6503.0
51.00	1710.0
52.00	153.0
56.00	604.0
57.00	1043.0
60.00	302.0
60.90	1372.0
62.00	1705.0
63.00	1277.0
63.90	109.0
65.10	139.0
68.00	2684.0
69.00	2821.0
70.00	296.0
72.10	155.0
73.00	1577.0
74.10	5121.0
75.00	14485.0
76.00	1270.0
76.90	198.0
78.90	1341.0
79.90	307.0
80.90	1145.0
81.80	291.0
86.90	946.0
88.00	1093.0
90.90	126.0
92.00	717.0
93.00	1285.0
94.00	3637.0
95.00	24528.0
96.00	1905.0
103.80	162.0
116.80	274.0
118.90	230.0
129.90	110.0
135.00	104.0
140.90	213.0
143.00	349.0
171.90	220.0
174.00	19328.0
175.00	1729.0
176.00	19368.0
177.10	1094.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	215.0
37.00	1777.0
38.00	1654.0
38.90	691.0
39.90	232.0
44.00	831.0
45.00	321.0
46.90	331.0
48.00	188.0
49.00	1221.0
50.00	6458.0
51.00	1698.0
51.90	117.0
56.00	563.0
57.00	972.0
60.00	251.0
60.90	1268.0
62.00	1543.0
63.00	1143.0
63.90	114.0
65.10	165.0
68.00	2675.0
69.00	2885.0
69.90	294.0
72.00	109.0
73.00	1542.0
74.10	4938.0
75.00	13965.0
76.00	1076.0
77.10	176.0
78.90	1303.0
79.90	326.0
80.90	1136.0
81.80	279.0
86.90	962.0
88.00	1020.0
90.90	107.0
92.00	724.0
93.00	1339.0
94.00	3500.0
95.00	23448.0
96.00	1806.0
103.80	160.0
116.80	215.0
117.70	103.0
118.80	215.0
130.00	103.0
140.90	217.0
143.00	386.0
172.00	207.0
174.00	18152.0
175.00	1614.0
176.00	19160.0
177.00	913.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Scan 2849 (10.250 min): VU034889.D
BFB41

m/z	Abundance
40.00	166.0
44.00	722.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41