
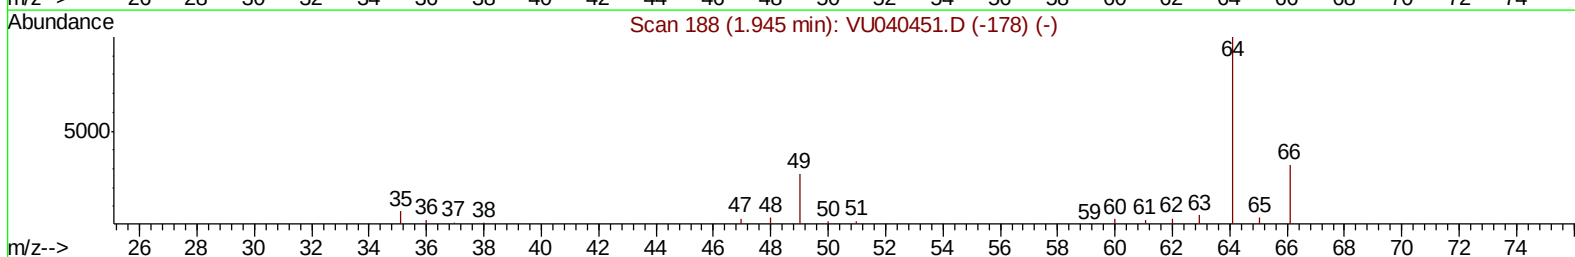
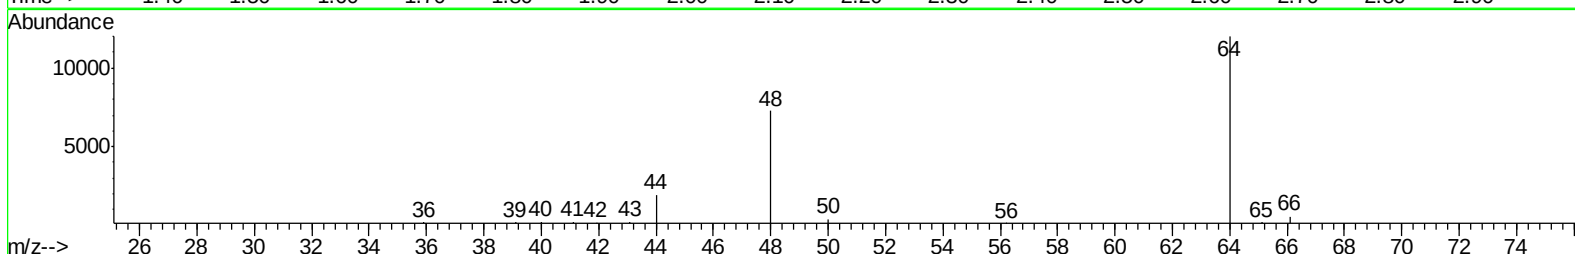


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100220\  
Data File : VU040461.D  
Acq On : 02 Oct 2020 15:19  
Operator : SY/MD  
Sample : L4240-08DL 10X  
Misc : 25.0mL/MSVOA U/WATER  
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Oct 03 02:15:51 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR092920WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Sat Oct 03 00:09:31 2020  
Response via : Initial Calibration

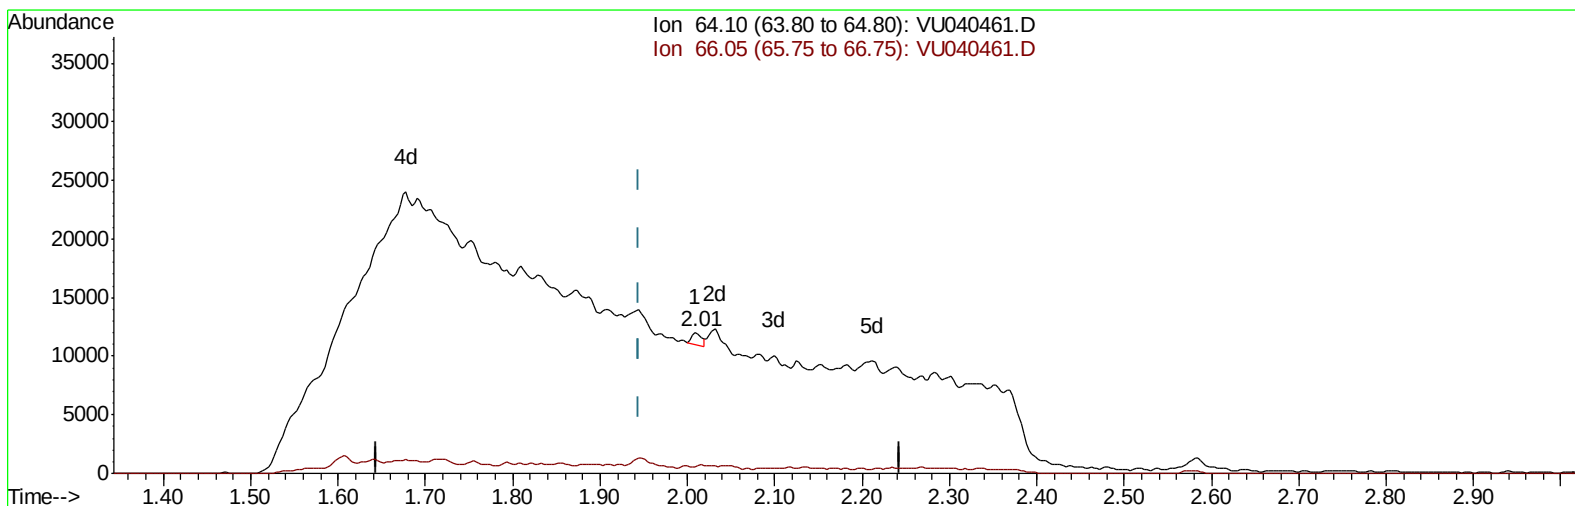

TIC: VU040461.D

(8) Chloroethane (T)

2.009min (+0.064) 0.11ug/L

response 822

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 64.10 | 100   | 100   |
| 66.05 | 30.50 | 4.36# |
| 0.00  | 0.00  | 0.00  |
| 0.00  | 0.00  | 0.00  |