
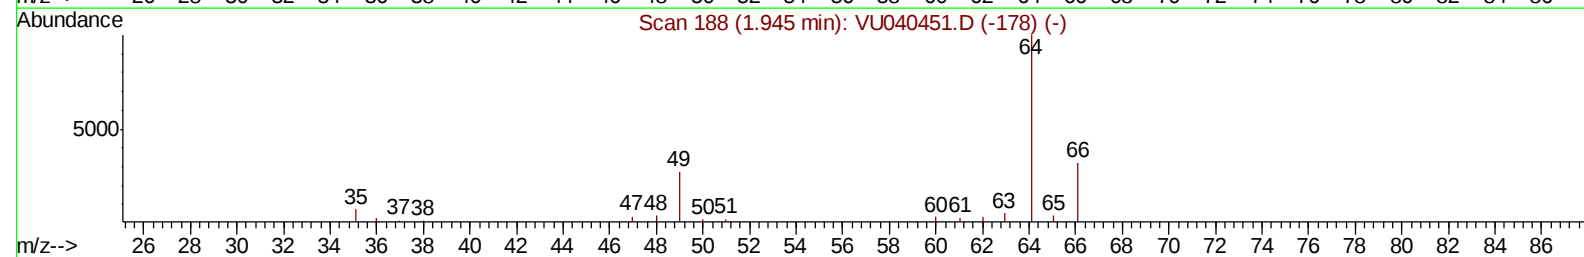
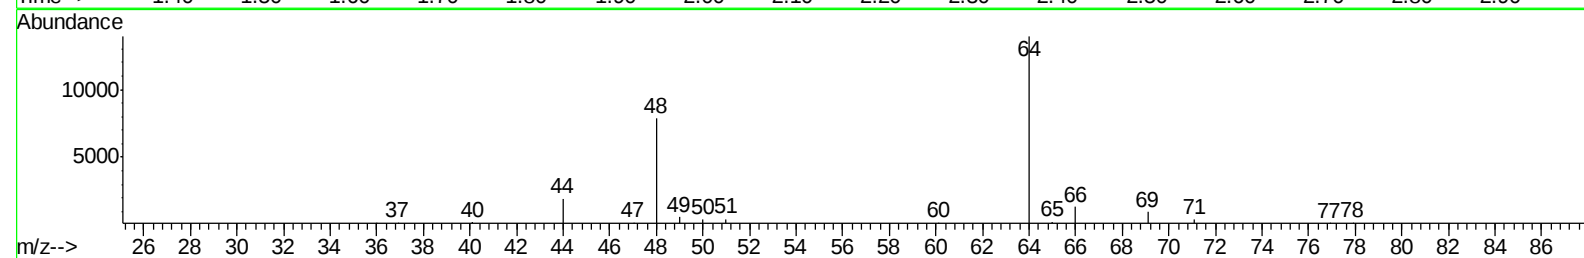


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100220\
 Data File : VU040461.D
 Acq On : 02 Oct 2020 15:19
 Operator : SY/MD
 Sample : L4240-08DL 10X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Oct 03 02:15:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 03 00:09:31 2020
 Response via : Initial Calibration

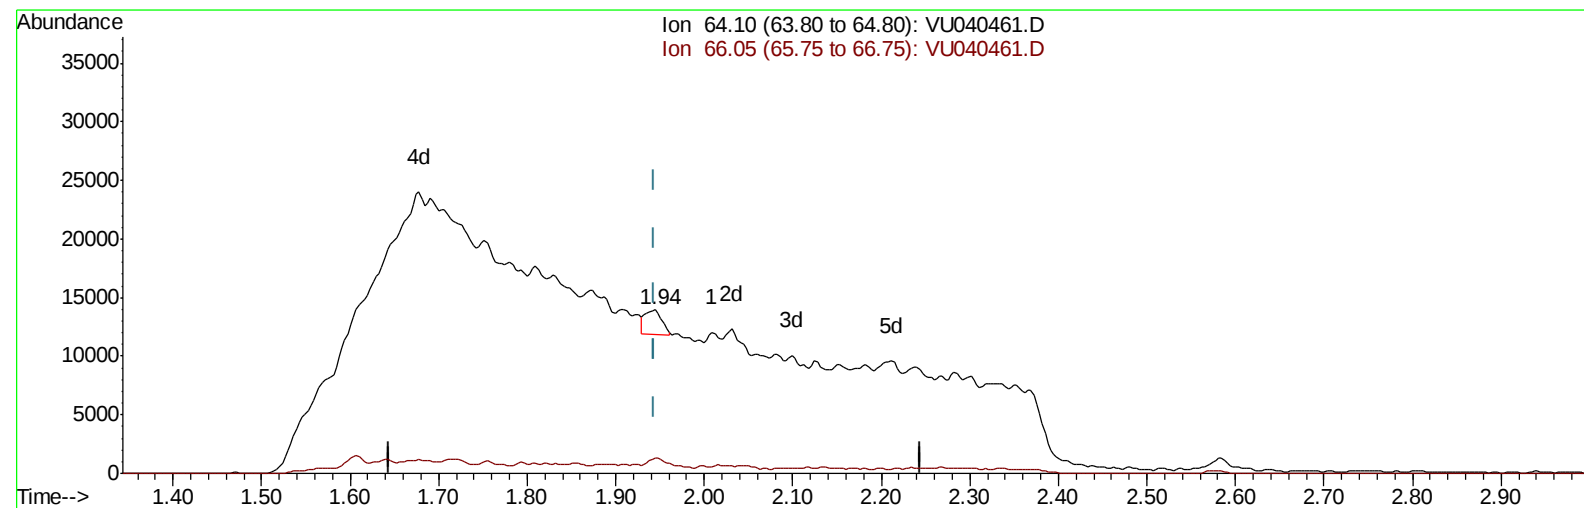

TIC: VU040461.D

(8) Chloroethane (T)

1.945min (+0.000) 0.35ug/L m

response 2695

Ion	Exp%	Act%
64.10	100	100
66.05	30.50	9.45#
0.00	0.00	0.00
0.00	0.00	0.00