




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
 Data File : VU055604.D
 Acq On : 02 Oct 2023 15:01
 Operator : MD/SY
 Sample : 04679-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB(20230928)

Manual IntegrationsAPPROVED

Quant Time: Oct 03 04:57:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 27 23:33:30 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/03/2023
 Supervised By :Semsettin Yesilyurt 10/03/2023

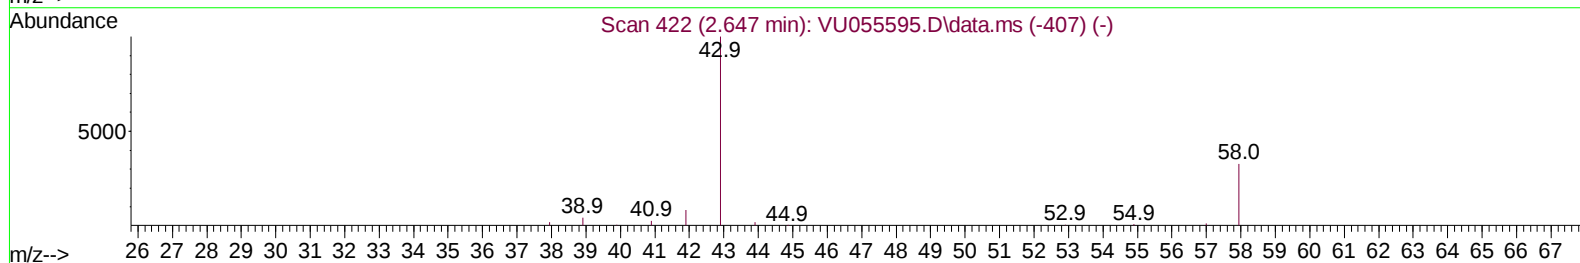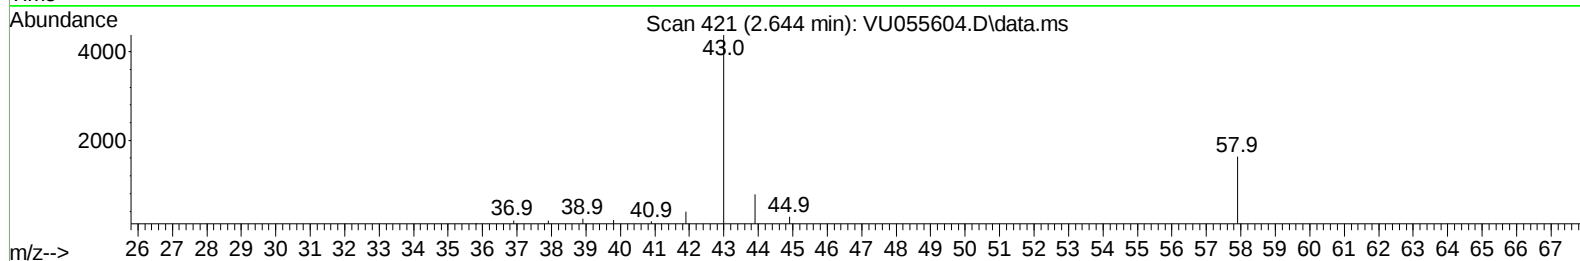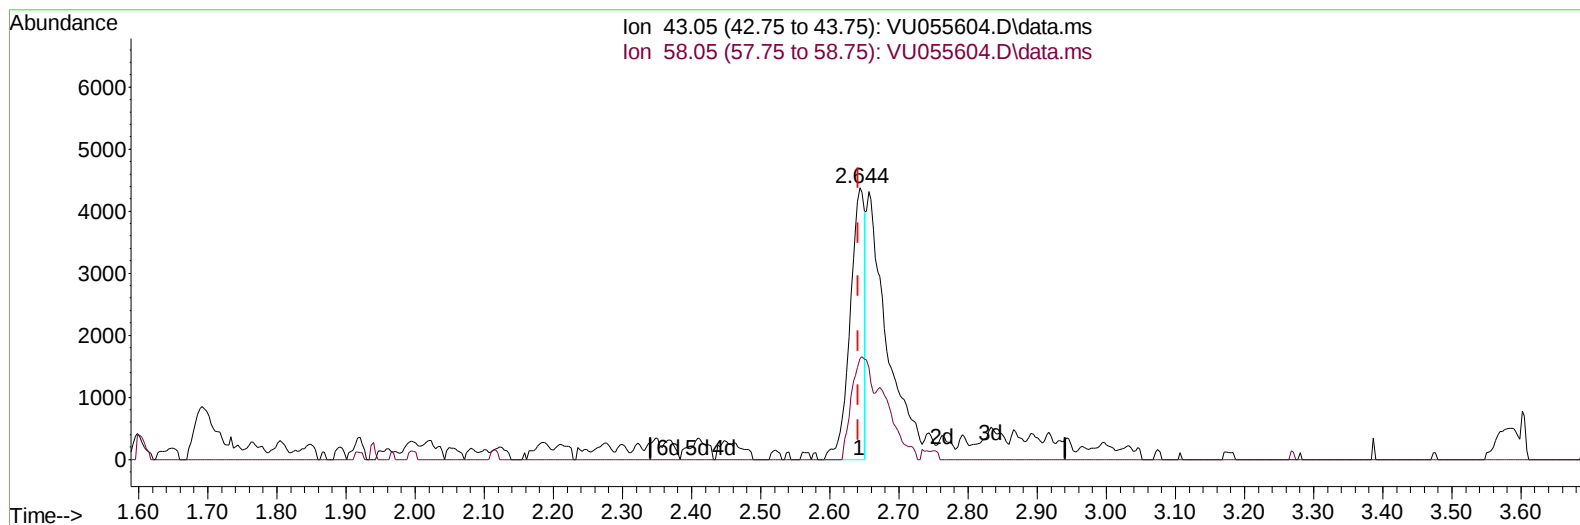

TIC: VU055604.D\data.ms

(13) Acetone (T)

2.644min (+ 0.003) 3.77 ug/L

response 6340

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	54.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
 Data File : VU055604.D
 Acq On : 02 Oct 2023 15:01
 Operator : MD/SY
 Sample : 04679-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB(20230928)

Manual IntegrationsAPPROVED

Quant Time: Oct 03 04:57:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 27 23:33:30 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/03/2023
 Supervised By :Semsettin Yesilyurt 10/03/2023

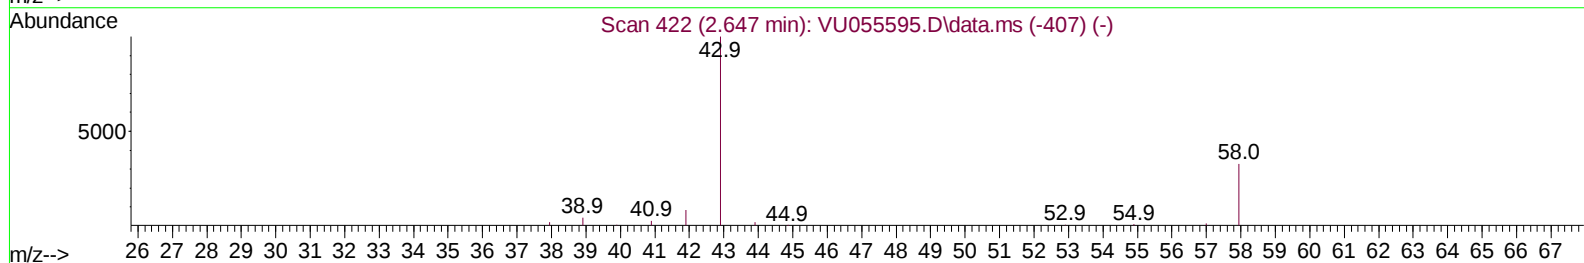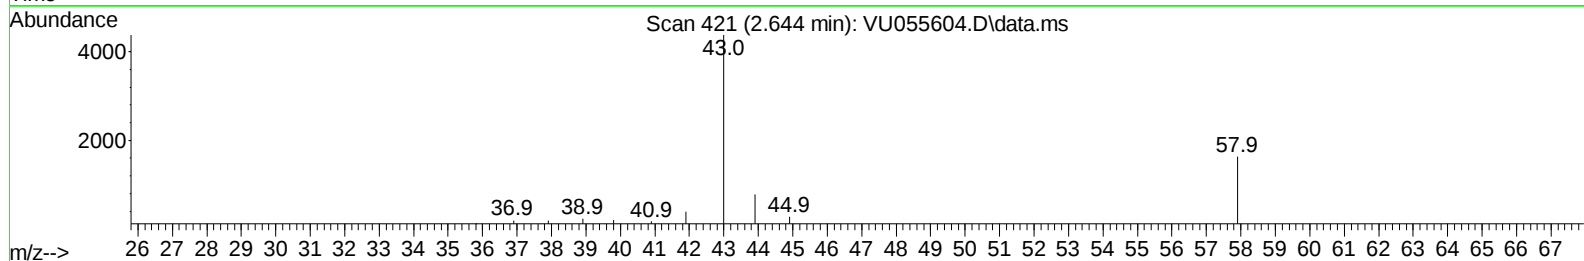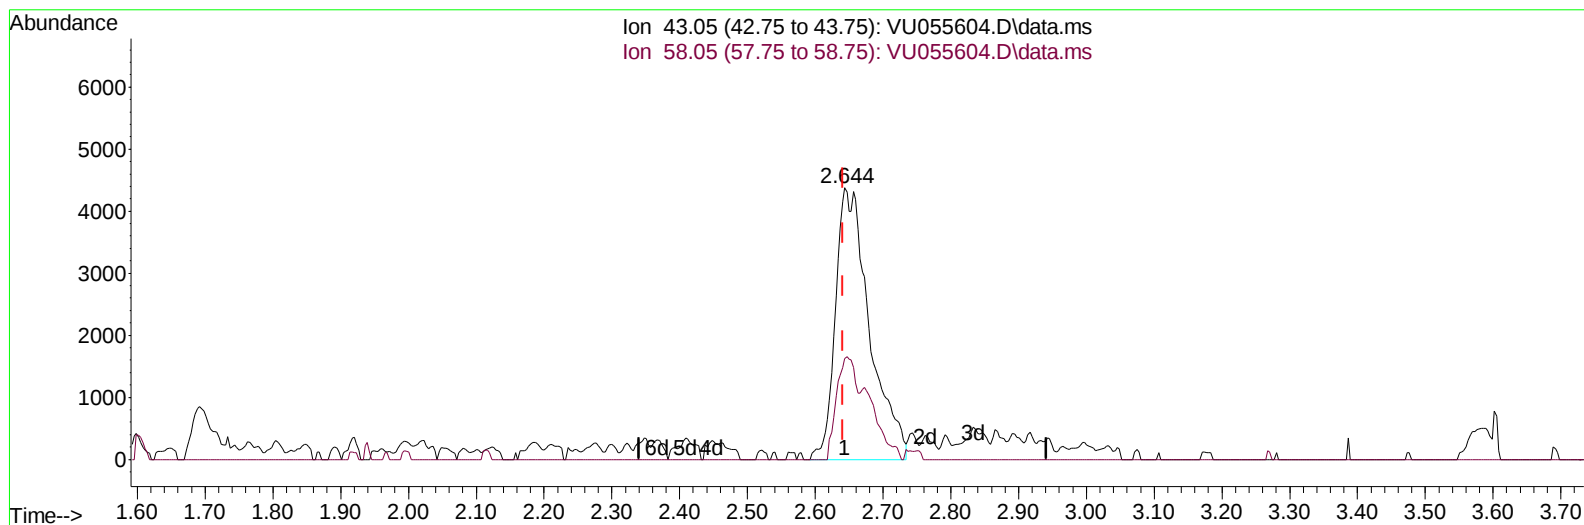

TIC: VU055604.D\data.ms

(13) Acetone (T)

2.644min (+ 0.003) 9.05 ug/L m

response 15238

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	22.67
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
 Data File : VU055604.D
 Acq On : 02 Oct 2023 15:01
 Operator : MD/SY
 Sample : 04679-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB(20230928)

Manual IntegrationsAPPROVED

Quant Time: Oct 03 04:57:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 27 23:33:30 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/03/2023
 Supervised By :Semsettin Yesilyurt 10/03/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.248	114		161725	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117		175662	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.810	152		84572	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.599	65		69649	4.261	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.200%	
7) Chloroethane-d5	1.914	69		70188	4.873	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.400%	
11) 1,1-Dichloroethene-d2	2.566	65		26097	3.879	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.600%	
20) 2-Butanone-d5	4.634	46		149226	50.545	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.080%	
24) Chloroform-d	5.061	84		136487	4.617	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%	
26) 1,2-Dichloroethane-d4	5.701	65		67888	4.774	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.400%	
32) Benzene-d6	5.727	84		250725	4.081	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.600%	
36) 1,2-Dichloropropane-d6	6.688	67		83879	4.569	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.400%	
41) Toluene-d8	7.897	98		218117	3.895	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.800%	
43) trans-1,3-Dichloroprop...	8.180	79		29277	4.544	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.800%	
46) 2-Hexanone-d5	8.634	63		84498	43.120	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.240%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84		63911	4.645	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.000%	
66) 1,2-Dichlorobenzene-d4	12.190	152		79259	4.643	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.800%	
Target Compounds							
13) Acetone	2.644	43		15238m	9.054	ug/L	
16) Methylene chloride	3.042	84		16272	1.201	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
Data File : VU055604.D
Acq On : 02 Oct 2023 15:01
Operator : MD/SY
Sample : 04679-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 3

Instrument :
MSVOA_U
ClientSampleId :
FB(20230928)

Manual IntegrationsAPPROVED

Quant Time: Oct 03 04:57:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 27 23:33:30 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/03/2023
Supervised By :Semsettin Yesilyurt 10/03/2023

