

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
 Data File : VU055596.D
 Acq On : 02 Oct 2023 11:14
 Operator : MD/SY
 Sample : VU1002WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK050

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	106	rBV	121352	132188	15.79%	1.979%
2	1.914	185	194	203	rBV	104976	136777	16.33%	2.047%
3	2.566	384	397	412	rBV	174847	288521	34.45%	4.319%
4	3.046	532	546	559	rBV4	15079	28090	3.35%	0.420%
5	4.634	1027	1040	1082	rBV	79482	302732	36.15%	4.531%
6	5.062	1157	1173	1199	rVB	172048	385237	46.00%	5.766%
7	5.724	1358	1379	1409	rBV2	313845	837407	100.00%	12.535%
8	6.248	1529	1542	1568	rBV	234775	466770	55.74%	6.987%
9	6.534	1621	1631	1641	rBV7	6875	13174	1.57%	0.197%
10	6.688	1663	1679	1699	rBV	199587	401873	47.99%	6.016%
11	7.566	1938	1952	1980	rBV	91130	174545	20.84%	2.613%
12	7.897	2041	2055	2081	rBV	373599	672212	80.27%	10.062%
13	8.180	2131	2143	2164	rBV	55225	100740	12.03%	1.508%
14	8.637	2273	2285	2323	rBV3	283686	715606	85.45%	10.712%
15	9.415	2515	2527	2549	rBV	347530	607314	72.52%	9.091%
16	10.756	2931	2944	2962	rBV	140897	234474	28.00%	3.510%
17	11.810	3260	3272	3293	rBV	355707	591410	70.62%	8.853%
18	12.193	3378	3391	3407	rBV	328977	553669	66.12%	8.288%
19	13.849	3897	3906	3919	rBV5	9256	14479	1.73%	0.217%
20	14.097	3974	3983	3997	rBV5	5567	10425	1.24%	0.156%
21	14.331	4048	4056	4069	rBV4	7922	12975	1.55%	0.194%




Sum of corrected areas: 6680618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
Data File : VU055596.D
Acq On : 02 Oct 2023 11:14
Operator : MD/SY
Sample : VU1002WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK050

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

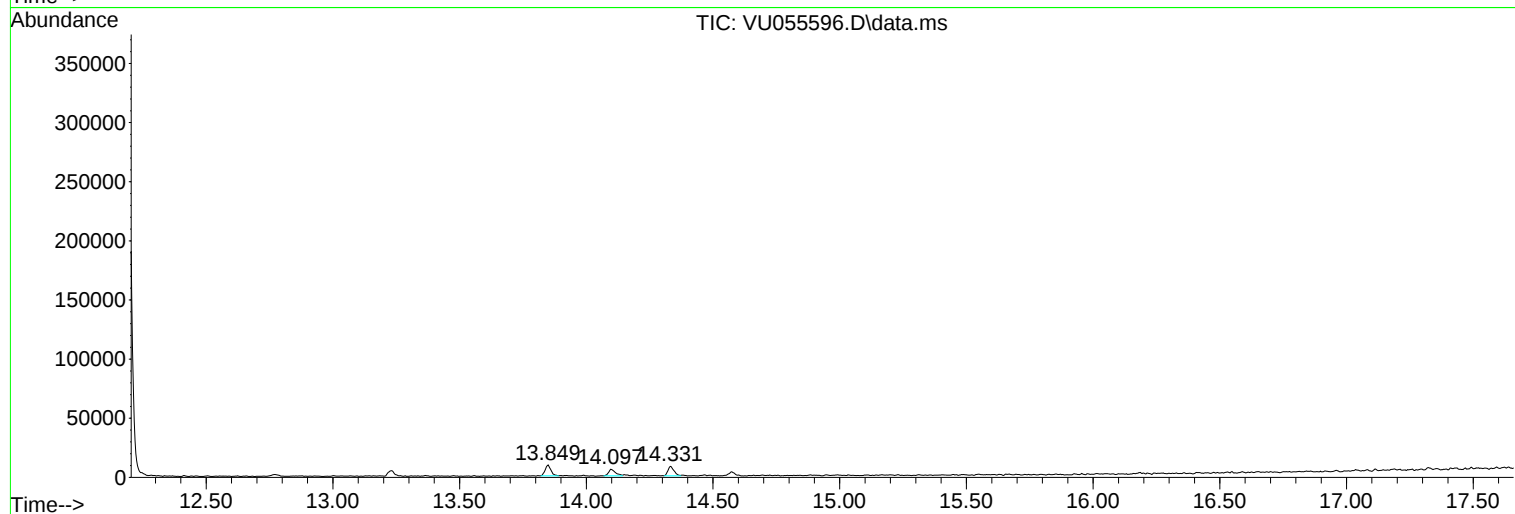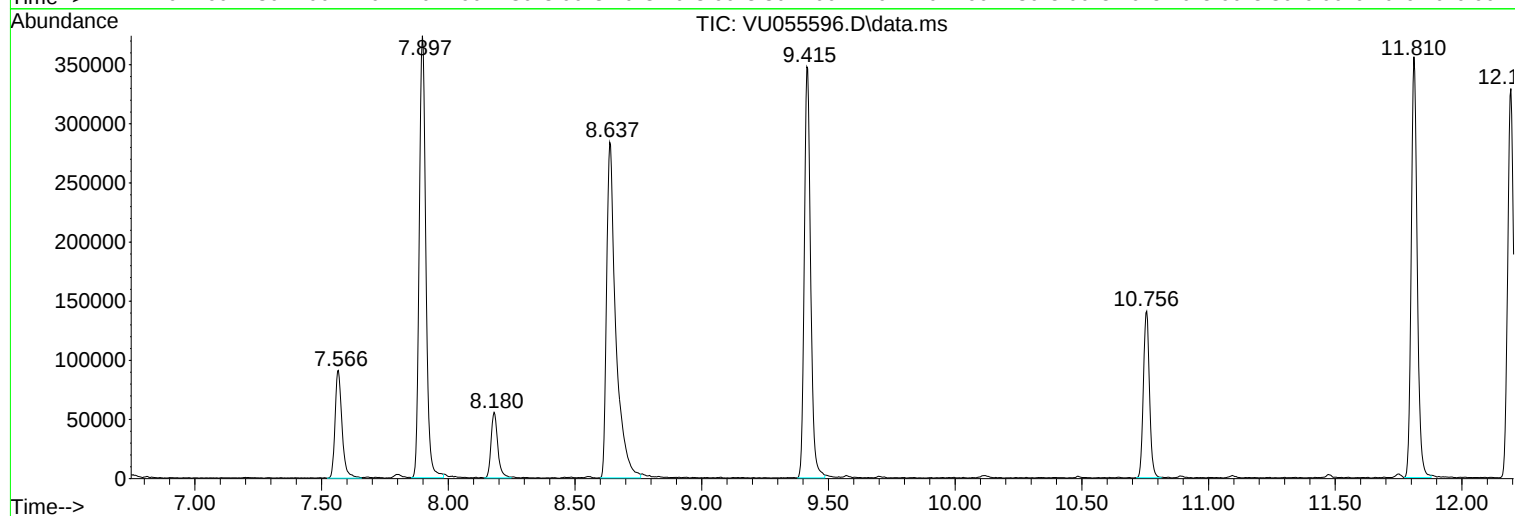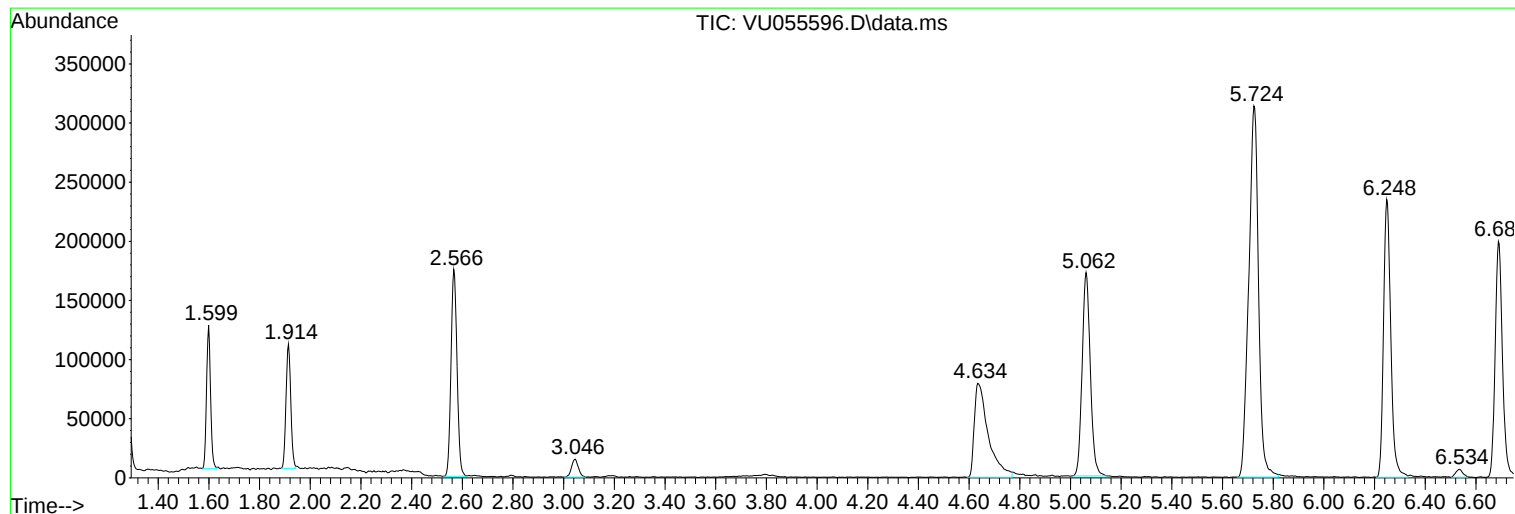

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
Data File : VU055596.D
Acq On : 02 Oct 2023 11:14
Operator : MD/SY
Sample : VU1002WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK050

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
Data File : VU055596.D
Acq On : 02 Oct 2023 11:14
Operator : MD/SY
Sample : VU1002WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK050

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------