

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
 Data File : VU055600.D
 Acq On : 02 Oct 2023 13:20
 Operator : MD/SY
 Sample : VIBLK147
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK147

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	111	rVB	109925	127262	15.26%	1.911%
2	1.914	185	194	207	rBV	105435	137141	16.44%	2.060%
3	2.567	385	397	417	rVB	168429	276433	33.14%	4.151%
4	3.046	534	546	562	rVB2	30311	55918	6.70%	0.840%
5	4.637	1027	1041	1094	rBV2	82356	318226	38.15%	4.779%
6	5.062	1157	1173	1198	rBV	170148	383819	46.01%	5.764%
7	5.724	1358	1379	1413	rBV2	315235	834218	100.00%	12.528%
8	6.248	1529	1542	1563	rBV	217563	429363	51.47%	6.448%
9	6.541	1617	1633	1650	rVB6	23824	49774	5.97%	0.747%
10	6.689	1665	1679	1699	rBV	194009	392876	47.10%	5.900%
11	7.566	1940	1952	1968	rBV	90263	167337	20.06%	2.513%
12	7.898	2041	2055	2077	rBV	368361	661356	79.28%	9.932%
13	8.181	2129	2143	2165	rBV2	57189	101287	12.14%	1.521%
14	8.637	2272	2285	2321	rBV3	296623	729078	87.40%	10.949%
15	9.415	2515	2527	2561	rBV	329126	574529	68.87%	8.628%
16	10.756	2930	2944	2959	rBV	149098	244135	29.27%	3.666%
17	10.891	2974	2986	3000	rBV4	8085	14497	1.74%	0.218%
18	11.811	3261	3272	3290	rBV	354190	587686	70.45%	8.826%
19	12.193	3377	3391	3413	rBV	337720	573916	68.80%	8.619%




Sum of corrected areas: 6658851

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
Data File : VU055600.D
Acq On : 02 Oct 2023 13:20
Operator : MD/SY
Sample : VIBLK147
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK147

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

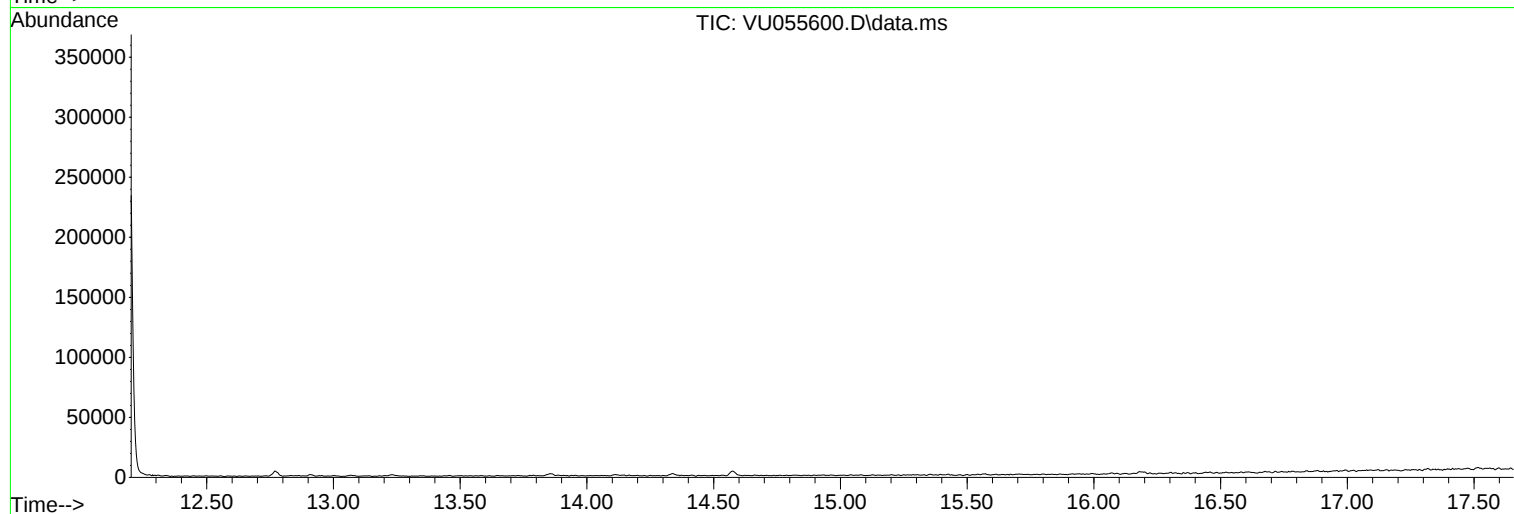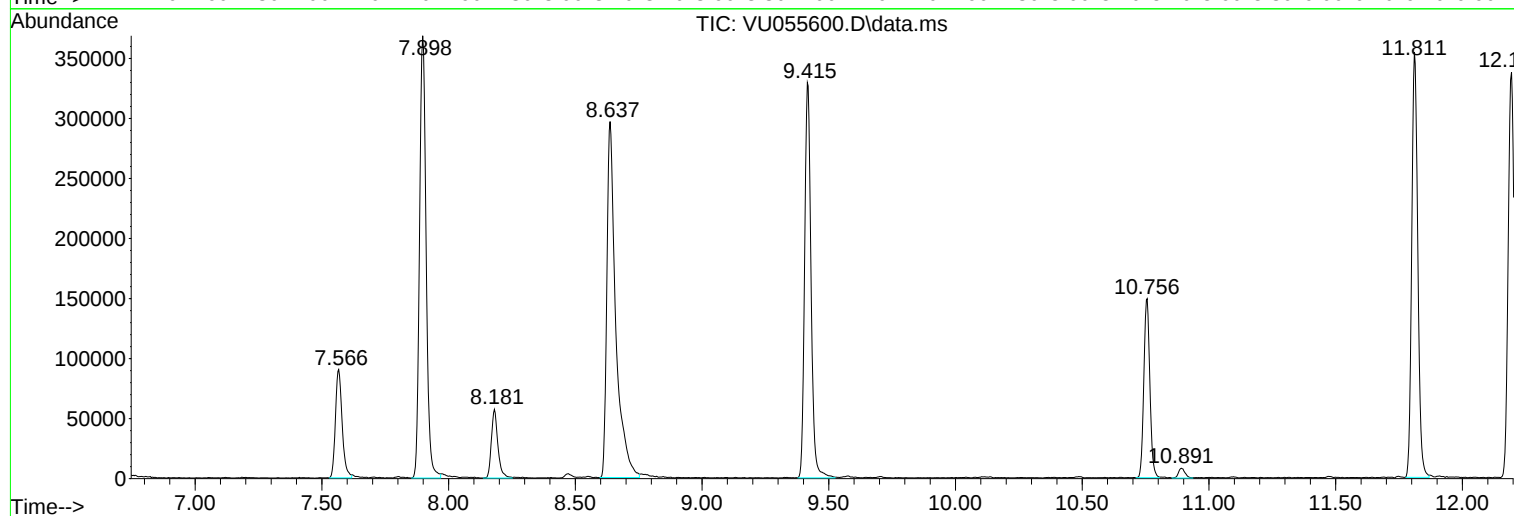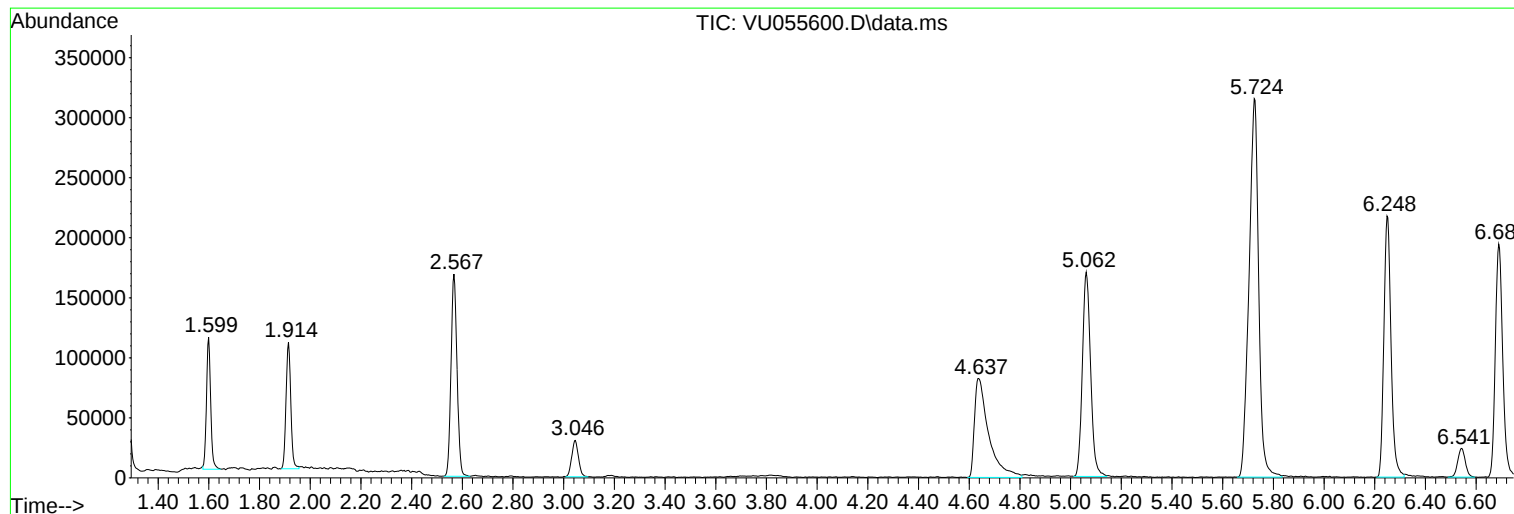

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
Data File : VU055600.D
Acq On : 02 Oct 2023 13:20
Operator : MD/SY
Sample : VIBLK147
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK147

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
Data File : VU055600.D
Acq On : 02 Oct 2023 13:20
Operator : MD/SY
Sample : VIBLK147
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK147

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc