


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100223\
Data File : VU055594.D
Acq On : 02 Oct 2023 08:37
Operator : MD/SY
Sample : BFB055
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB055

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Oct 03 06:03:59 2023

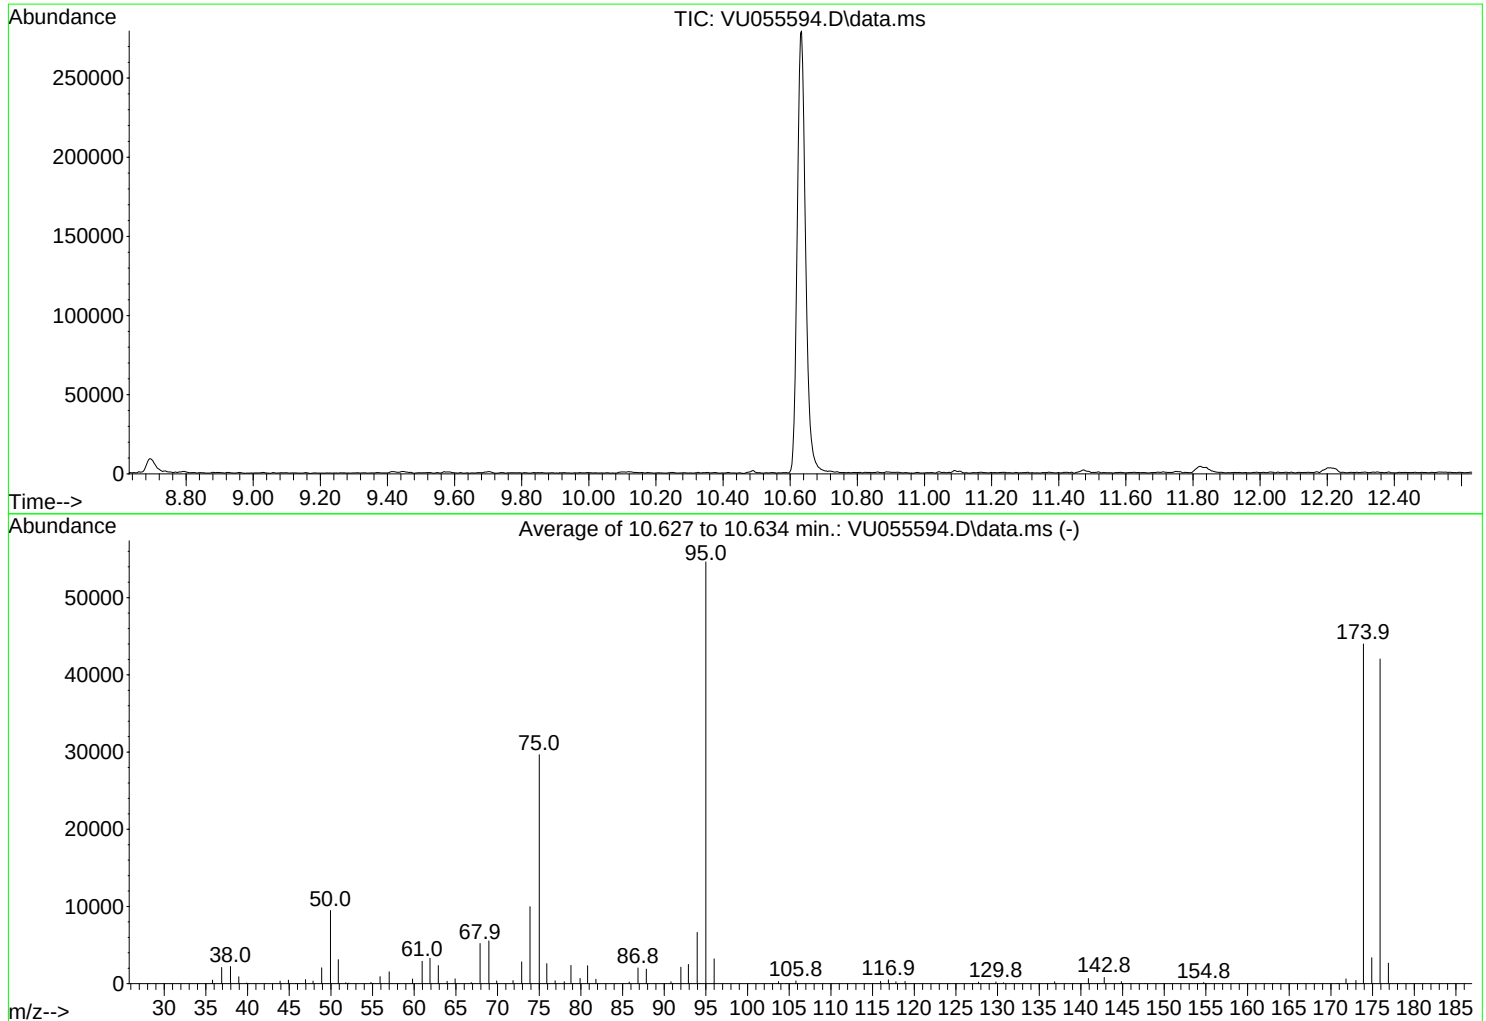

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	9476	PASS
75	95	30	80	54.3	29672	PASS
95	95	100	100	100.0	54643	PASS
96	95	5	9	5.9	3217	PASS
173	174	0.00	2	0.9	412	PASS
174	95	50	120	80.5	43997	PASS
175	174	5	9	7.6	3361	PASS
176	174	95	101	95.6	42059	PASS
177	176	5	9	6.3	2655	PASS

m/z	Abundance
35.70	113.0
39.90	117.0
43.90	562.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
35.80	579.0
36.90	2045.0
38.00	2189.0
38.90	966.0
39.90	160.0
43.90	842.0
44.90	412.0
45.80	111.0
47.00	518.0
47.80	318.0
48.90	1842.0
49.90	8999.0
50.90	2924.0
52.10	170.0
54.80	193.0
55.90	832.0
57.00	1463.0
59.80	560.0
60.90	3052.0
61.90	3258.0
62.90	2240.0
64.00	288.0
64.90	564.0
66.90	153.0
67.90	4932.0
69.00	5492.0
69.90	309.0
71.90	324.0
72.90	2622.0
73.90	9676.0
75.00	27808.0
75.90	2542.0
76.90	407.0
78.00	230.0
78.80	2030.0
79.90	717.0
80.80	2089.0
81.80	592.0
85.80	200.0
86.90	1823.0
87.90	1786.0
90.80	208.0
92.00	1893.0
92.90	2226.0
93.90	6264.0
95.00	52024.0
96.00	3237.0
103.70	286.0
105.80	331.0
116.00	269.0
116.90	454.0
117.80	204.0
118.90	297.0
127.70	259.0
129.80	230.0
136.90	180.0
140.90	659.0
142.80	754.0
144.80	231.0
154.70	137.0
171.80	579.0
173.00	374.0
173.90	40360.0
174.90	3126.0
175.90	37824.0
176.90	2442.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
35.90	571.0
36.90	2120.0
37.90	2243.0
38.90	900.0
39.90	183.0
43.90	950.0
44.90	468.0
47.00	527.0
47.90	336.0
48.90	2086.0
49.90	9813.0
50.90	3254.0
51.80	196.0
54.80	165.0
55.90	939.0
57.00	1602.0
59.80	630.0
60.90	2976.0
61.90	3387.0
62.90	2436.0
63.90	283.0
64.90	657.0
66.80	151.0
67.90	5277.0
69.00	5705.0
69.90	335.0
71.80	428.0
72.90	2916.0
73.90	10241.0
75.00	30656.0
75.90	2650.0
76.90	375.0
78.00	249.0
78.80	2412.0
79.90	703.0
80.80	2430.0
81.80	598.0
85.80	230.0
86.80	2006.0
87.90	1909.0
90.80	266.0
92.00	2253.0
92.90	2550.0
94.00	6832.0
95.00	55960.0
96.00	3269.0
103.70	284.0
105.80	364.0
116.00	286.0
116.90	531.0
117.80	288.0
118.90	292.0
127.70	191.0
129.80	230.0
130.70	160.0
136.80	273.0
140.90	694.0
142.80	845.0
144.90	264.0
154.80	168.0
171.80	626.0
173.00	431.0
173.90	45512.0
174.90	3474.0
175.90	43560.0
176.90	2698.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
35.90	563.0
36.90	2130.0
37.90	2232.0
39.00	789.0
39.90	229.0
43.90	922.0
44.90	470.0
46.90	484.0
47.90	337.0
48.90	2252.0
50.00	9615.0
50.90	3124.0
51.80	186.0
54.80	133.0
55.90	977.0
57.00	1565.0
59.80	633.0
61.00	2681.0
61.90	3237.0
62.90	2354.0
63.90	370.0
64.90	646.0
66.80	116.0
67.90	5398.0
68.90	5403.0
69.90	387.0
71.80	424.0
72.90	2916.0
73.90	9994.0
75.00	30552.0
75.90	2555.0
76.90	328.0
78.00	270.0
78.80	2639.0
79.90	633.0
80.80	2463.0
81.80	539.0
85.80	185.0
86.80	2287.0
87.80	1980.0
90.80	255.0
92.00	2274.0
92.90	2665.0
94.00	6833.0
95.00	55944.0
96.00	3144.0
103.70	271.0
104.70	107.0
105.80	368.0
115.90	323.0
116.90	512.0
117.80	268.0
118.90	299.0
127.70	144.0
129.80	212.0
130.70	187.0
136.80	299.0
140.90	617.0
142.80	838.0
144.80	305.0
145.90	110.0
147.70	116.0
154.80	181.0
170.80	107.0
171.80	689.0
173.00	432.0
173.90	46120.0
174.90	3483.0
175.90	44792.0
176.90	2824.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055