

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
 Data File : VU061070.D
 Acq On : 02 Oct 2024 12:47
 Operator : MD/SY
 Sample : P4227-04 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-9D(20240926)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	110	rVB	76905	87212	6.32%	1.182%
2	1.911	185	193	206	rBV	59549	79082	5.73%	1.072%
3	2.560	384	395	417	rVB	122701	203597	14.74%	2.759%
4	3.177	573	587	605	rBV2	14279	32697	2.37%	0.443%
5	4.631	1020	1039	1066	rBV3	101367	296208	21.45%	4.014%
6	5.052	1155	1170	1193	rBV	107067	243788	17.65%	3.304%
7	5.717	1356	1377	1405	rBV2	224436	595382	43.11%	8.068%
8	6.242	1526	1540	1573	rBV	224488	452365	32.76%	6.130%
9	6.682	1662	1677	1704	rBV	144916	290229	21.02%	3.933%
10	7.560	1939	1950	1970	rBV	77546	147141	10.65%	1.994%
11	7.891	2041	2053	2082	rBV	278935	505077	36.57%	6.845%
12	8.174	2131	2141	2164	rBV	44969	85449	6.19%	1.158%
13	8.627	2269	2282	2313	rBV	329591	665035	48.16%	9.012%
14	9.412	2513	2526	2556	rBV	312915	623127	45.12%	8.444%
15	10.746	2928	2941	2959	rBV	99024	164842	11.94%	2.234%
16	11.740	3239	3250	3260	rBV	71954	117145	8.48%	1.588%
17	11.804	3260	3270	3298	rVB2	347108	903413	65.42%	12.243%
18	12.183	3376	3388	3414	rBV	248598	449143	32.52%	6.087%
19	13.830	3888	3900	3934	rBV	831037	1380962	100.00%	18.714%
20	14.325	4044	4054	4070	rBV3	33324	57244	4.15%	0.776%

Sum of corrected areas: 7379138




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
Data File : VU061070.D
Acq On : 02 Oct 2024 12:47
Operator : MD/SY
Sample : P4227-04 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-9D(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

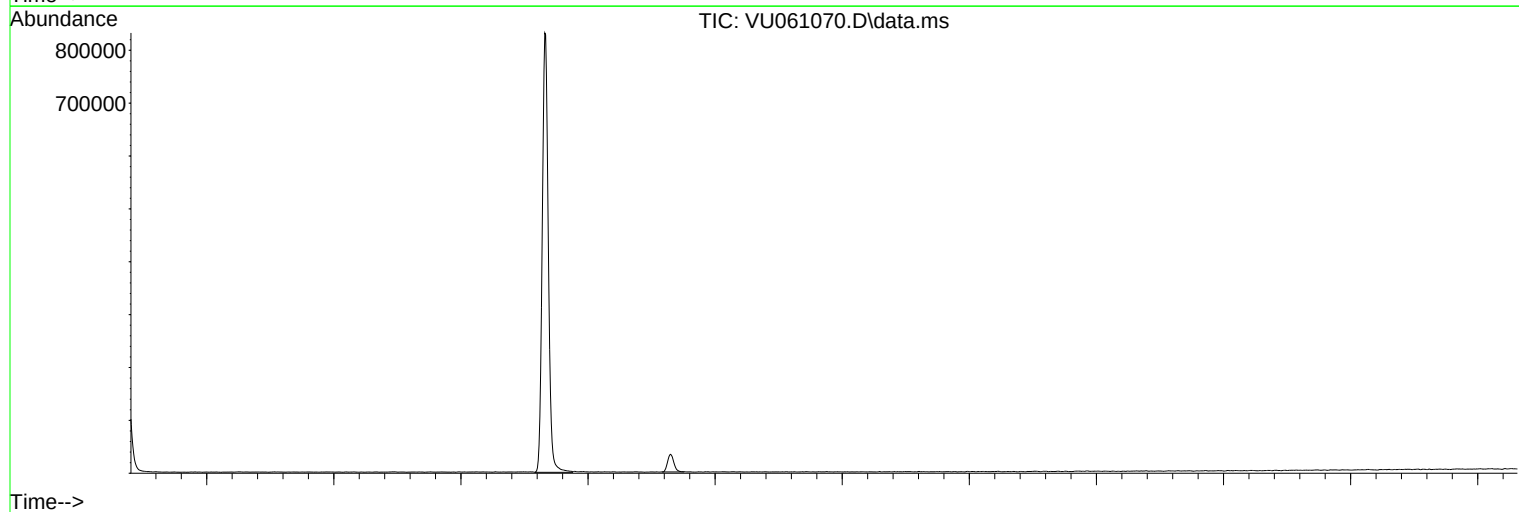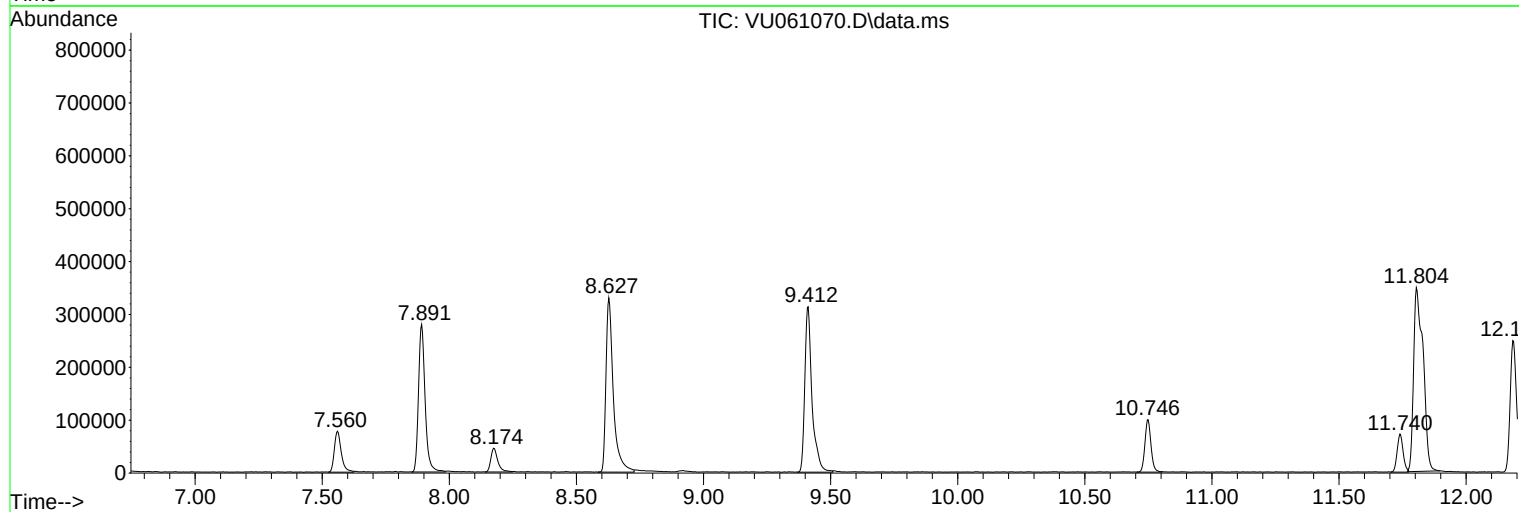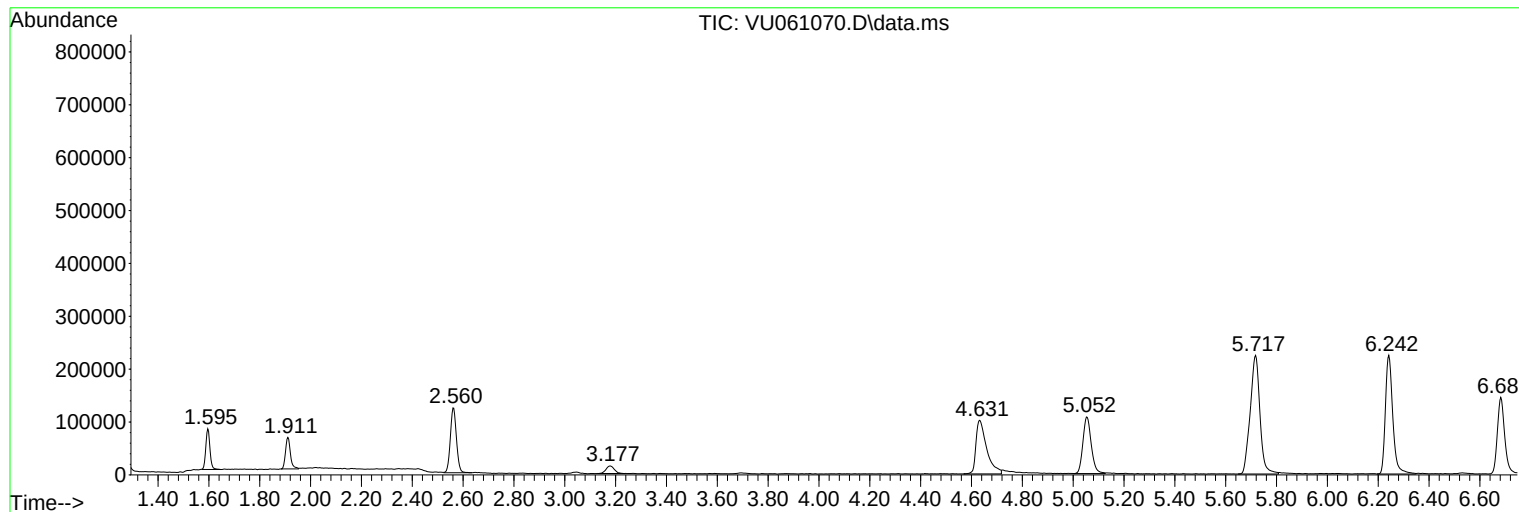

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
Data File : VU061070.D
Acq On : 02 Oct 2024 12:47
Operator : MD/SY
Sample : P4227-04 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-9D(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
Data File : VU061070.D
Acq On : 02 Oct 2024 12:47
Operator : MD/SY
Sample : P4227-04 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-9D(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------