

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
 Data File : VU061074.D
 Acq On : 02 Oct 2024 14:25
 Operator : MD/SY
 Sample : P4227-07 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DUP(20240926)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	108	rVB	76675	86506	3.04%	0.961%
2	1.911	185	193	204	rBV	57690	74692	2.63%	0.829%
3	2.563	383	396	410	rVB	119802	196634	6.91%	2.184%
4	3.177	572	587	604	rBV	17107	40003	1.41%	0.444%
5	4.631	1021	1039	1079	rBV2	103257	317860	11.17%	3.530%
6	5.055	1156	1171	1195	rBV	106768	241976	8.51%	2.687%
7	5.718	1357	1377	1409	rBV2	218279	582832	20.49%	6.472%
8	6.242	1528	1540	1571	rBV	211855	424976	14.94%	4.719%
9	6.682	1663	1677	1702	rBV	140725	284414	10.00%	3.158%
10	7.560	1935	1950	1973	rBV	75331	142567	5.01%	1.583%
11	7.891	2041	2053	2074	rBV	269979	493262	17.34%	5.478%
12	8.174	2131	2141	2166	rBV	44448	82465	2.90%	0.916%
13	8.627	2271	2282	2319	rBV	324401	663686	23.33%	7.370%
14	9.438	2529	2534	2562	rVB	629215	1073537	37.73%	11.922%
15	10.749	2930	2942	2962	rBV	94707	159743	5.61%	1.774%
16	11.740	3238	3250	3261	rBV	451177	753911	26.50%	8.372%
17	11.827	3261	3277	3308	rVB2	1453905	2845030	100.00%	31.594%
18	12.187	3375	3389	3420	rBV2	255485	495356	17.41%	5.501%
19	13.843	3894	3904	3924	rBV2	22941	45468	1.60%	0.505%

Sum of corrected areas: 9004918




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
Data File : VU061074.D
Acq On : 02 Oct 2024 14:25
Operator : MD/SY
Sample : P4227-07 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

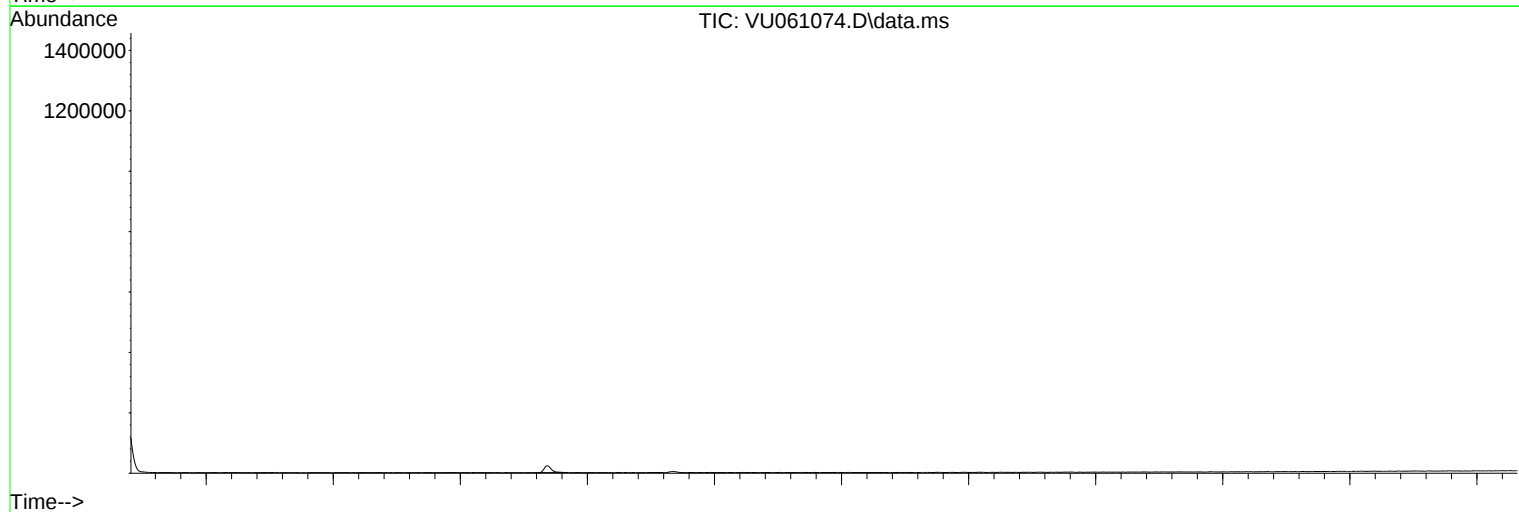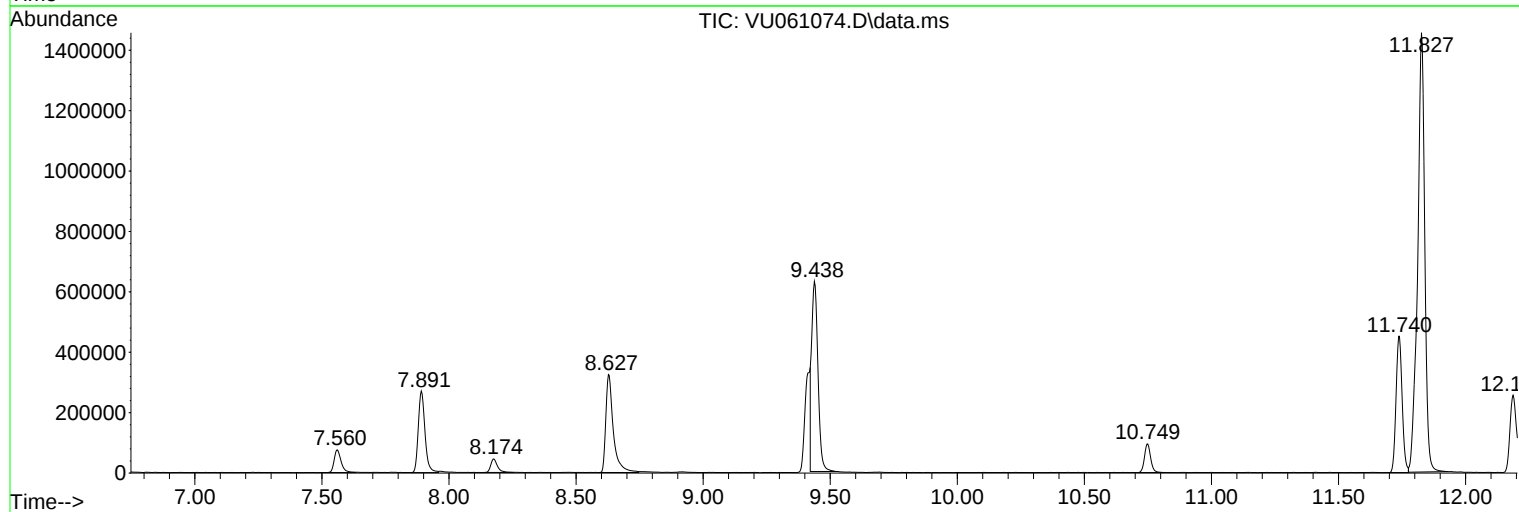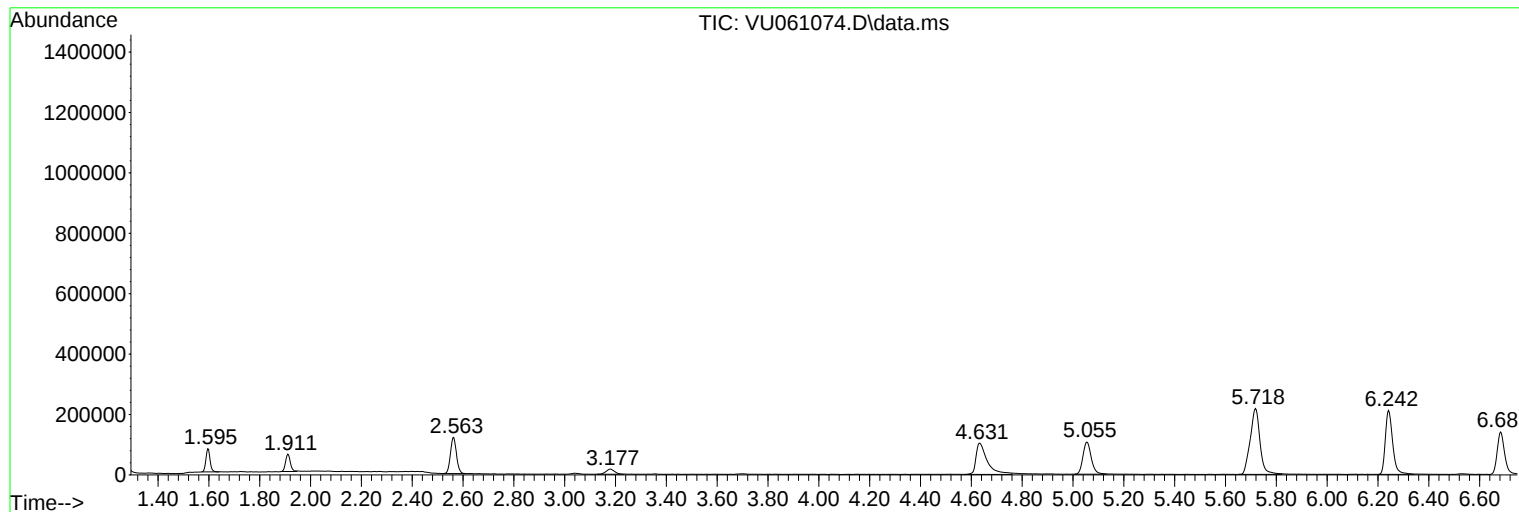

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
Data File : VU061074.D
Acq On : 02 Oct 2024 14:25
Operator : MD/SY
Sample : P4227-07 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
Data File : VU061074.D
Acq On : 02 Oct 2024 14:25
Operator : MD/SY
Sample : P4227-07 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP(20240926)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------