

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
 Data File : VU061078.D
 Acq On : 02 Oct 2024 15:59
 Operator : MD/SY
 Sample : VIBLK145
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK145

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	104	rBV	74992	84742	13.03%	1.642%
2	1.911	185	193	205	rBV	58171	76712	11.80%	1.487%
3	2.563	384	396	412	rVB	120544	199623	30.70%	3.868%
4	4.634	1030	1040	1073	rBV	80980	236722	36.41%	4.587%
5	5.055	1156	1171	1199	rBV	106195	242690	37.33%	4.703%
6	5.718	1357	1377	1412	rBV2	218861	582774	89.63%	11.293%
7	6.242	1526	1540	1570	rBV	216900	429511	66.06%	8.323%
8	6.682	1664	1677	1703	rBV	136374	278021	42.76%	5.388%
9	7.560	1938	1950	1974	rBV2	75402	144514	22.23%	2.800%
10	7.891	2040	2053	2083	rBV	266577	496610	76.38%	9.623%
11	8.174	2131	2141	2159	rBV	44526	83712	12.88%	1.622%
12	8.627	2272	2282	2314	rBV	308356	650164	100.00%	12.599%
13	9.412	2513	2526	2551	rBV	294752	530636	81.62%	10.283%
14	10.746	2930	2941	2961	rBV	92036	158676	24.41%	3.075%
15	11.743	3243	3251	3260	rBV2	5979	9523	1.46%	0.185%
16	11.804	3260	3270	3297	rVV	293762	527054	81.06%	10.213%
17	12.187	3377	3389	3414	rBV	225557	399841	61.50%	7.748%
18	13.849	3896	3906	3917	rBV6	8054	14359	2.21%	0.278%
19	14.328	4045	4055	4070	rVB3	8481	14522	2.23%	0.281%

Sum of corrected areas: 5160406




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
Data File : VU061078.D
Acq On : 02 Oct 2024 15:59
Operator : MD/SY
Sample : VIBLK145
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

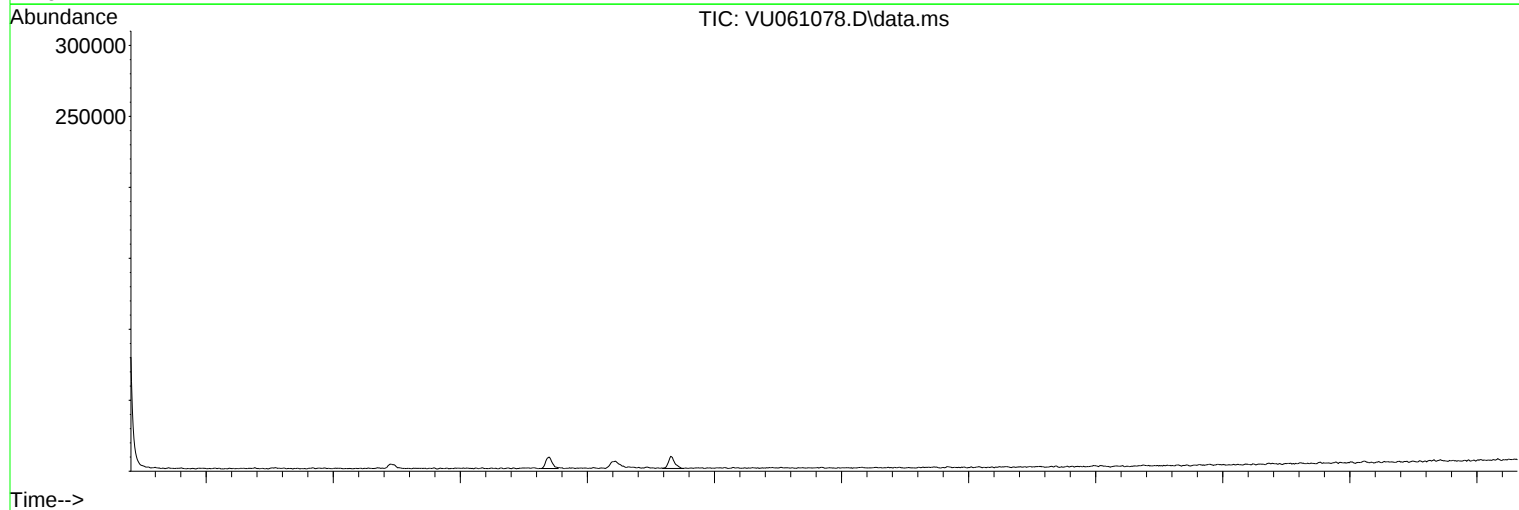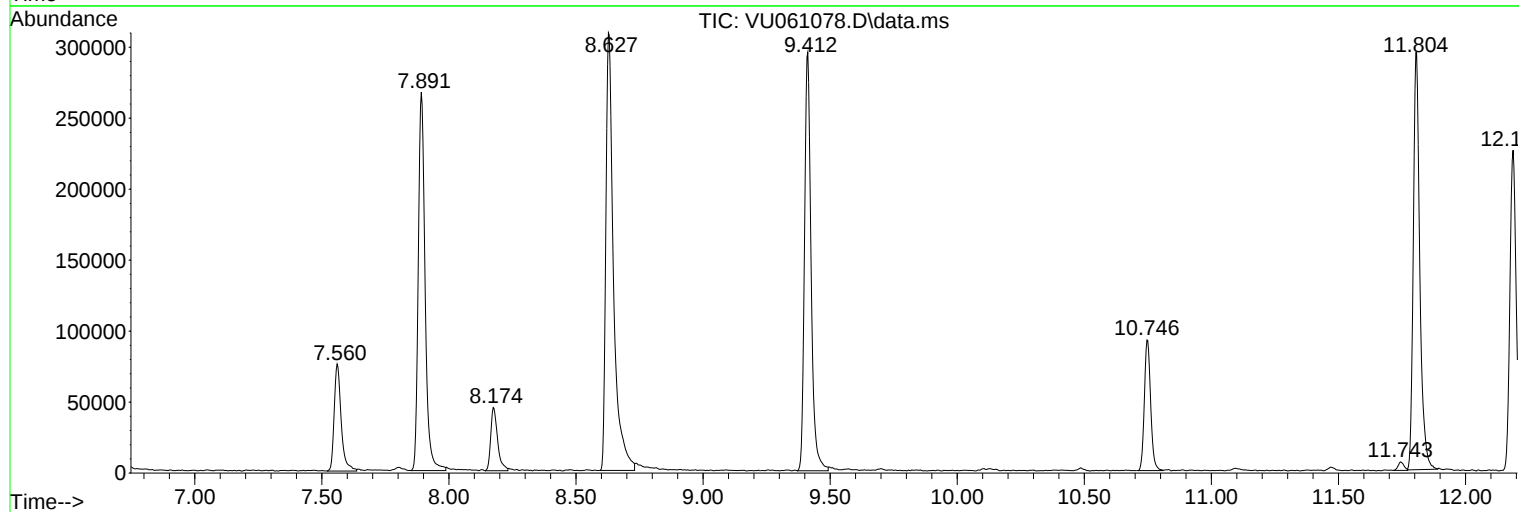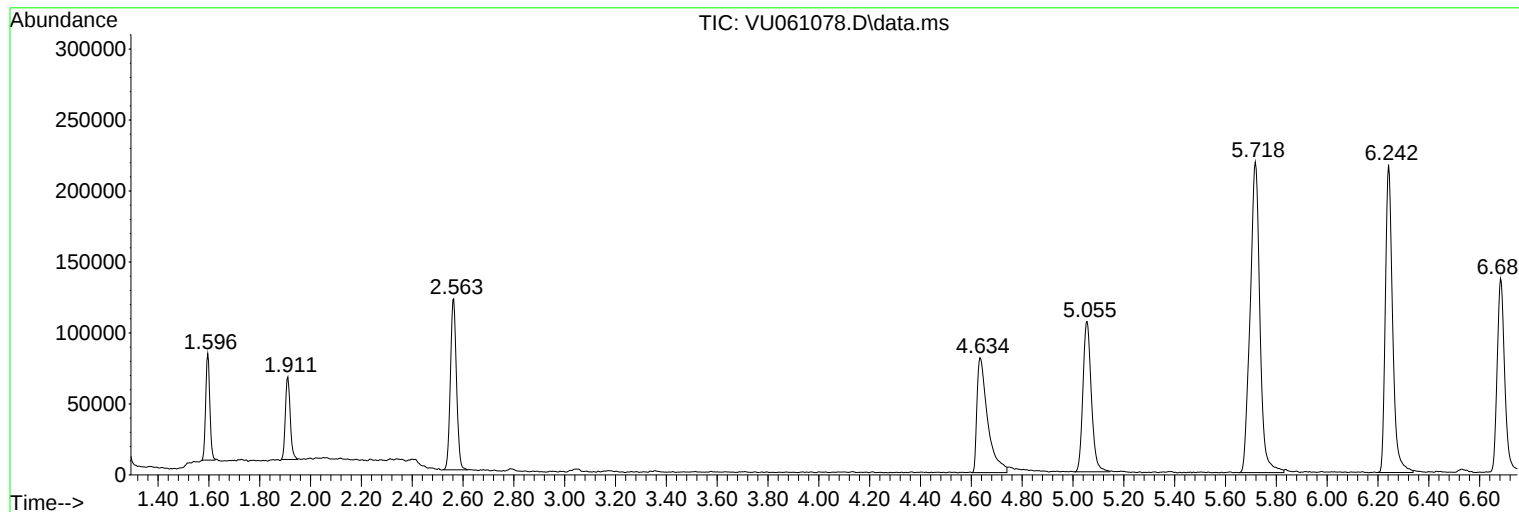

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
Data File : VU061078.D
Acq On : 02 Oct 2024 15:59
Operator : MD/SY
Sample : VIBLK145
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
Data File : VU061078.D
Acq On : 02 Oct 2024 15:59
Operator : MD/SY
Sample : VIBLK145
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
