
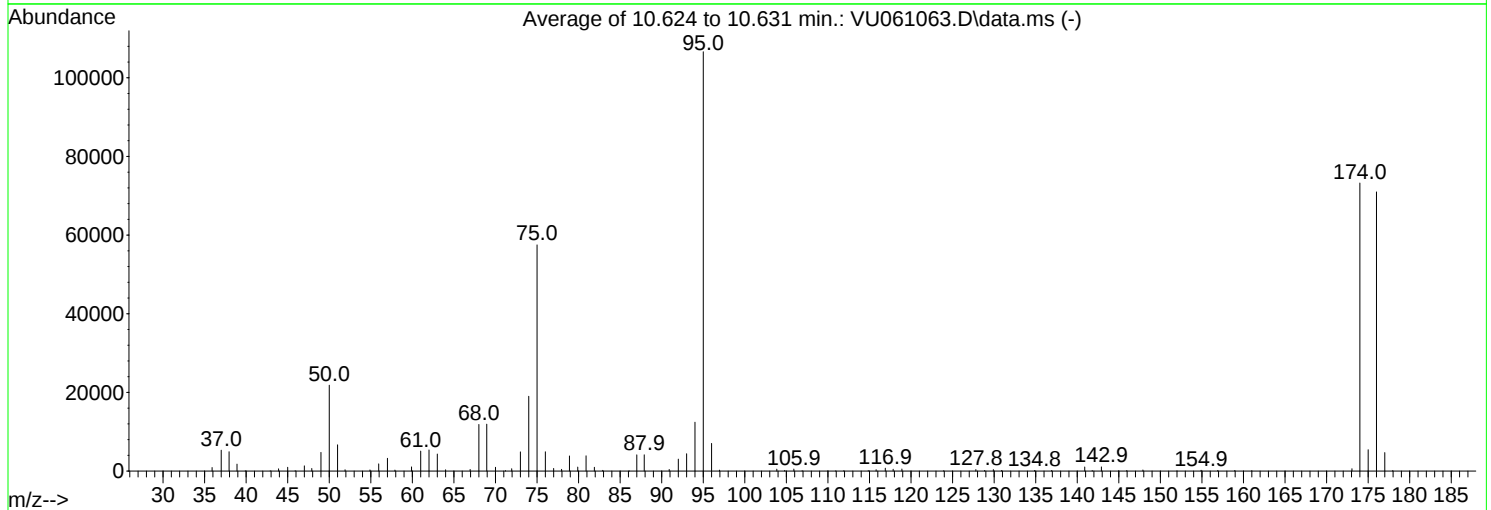


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100224\
Data File : VU061063.D
Acq On : 02 Oct 2024 09:13
Operator : MD/SY
Sample : BFB009
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB009

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Oct 03 06:26:52 2024

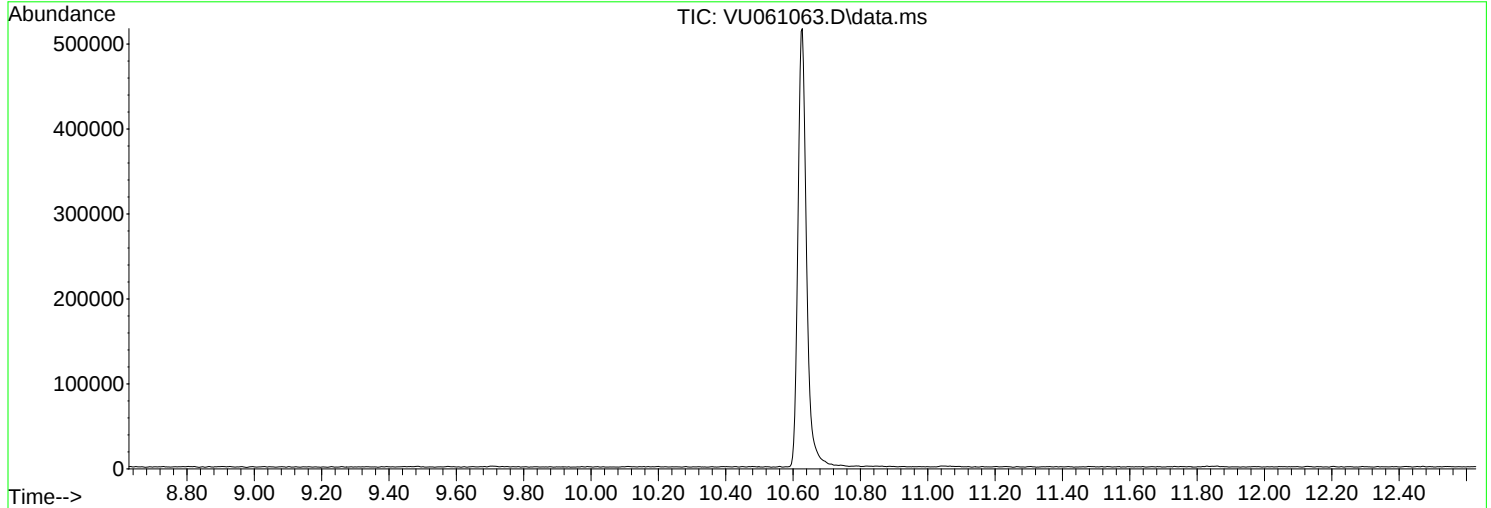

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	21840	PASS
75	95	30	80	53.9	57515	PASS
95	95	100	100	100.0	106624	PASS
96	95	5	9	6.6	7033	PASS
173	174	0.00	2	0.8	601	PASS
174	95	50	120	68.7	73237	PASS
175	174	5	9	7.4	5434	PASS
176	174	95	101	96.9	70984	PASS
177	176	5	9	6.6	4700	PASS

m/z	Abundance
38.90	130.0
39.90	191.0
40.90	244.0
42.00	117.0
42.90	314.0
43.90	767.0
54.90	189.0
56.00	143.0
57.00	156.0
68.90	101.0
70.90	109.0
85.00	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
35.90	870.0
37.00	5408.0
37.90	5257.0
39.00	1986.0
39.90	270.0
41.00	216.0
41.90	102.0
42.90	346.0
43.90	1318.0
45.00	980.0
47.00	1361.0
47.90	639.0
49.00	5021.0
50.00	22728.0
51.00	6972.0
51.90	402.0
54.90	519.0
55.90	2026.0
57.00	3555.0
57.90	258.0
59.90	1026.0
61.00	5211.0
62.00	5512.0
63.00	4430.0
64.00	338.0
67.00	452.0
68.00	12497.0
69.00	12452.0
70.00	981.0
71.20	176.0
71.90	638.0
73.00	5165.0
74.00	19808.0
75.00	59160.0
76.00	5151.0
77.00	780.0
78.00	436.0
78.90	4002.0
79.90	1032.0
80.90	4083.0
81.90	950.0
82.90	196.0
87.00	4317.0
87.90	4080.0
90.90	449.0
92.00	3171.0
93.00	4531.0
94.00	12772.0
95.00	109384.0
96.00	7212.0
97.00	267.0
103.90	496.0
104.80	152.0
105.90	512.0
106.90	152.0
111.90	107.0
114.80	117.0
115.80	353.0
116.90	712.0
117.90	439.0
118.90	513.0
123.90	109.0
127.80	420.0
128.90	191.0
129.90	386.0
131.00	187.0
134.90	187.0
136.80	141.0
140.90	1007.0
141.80	137.0
142.90	1111.0
145.00	128.0
145.90	128.0
147.90	291.0
154.90	227.0
156.90	166.0
159.00	154.0
161.00	127.0
173.00	640.0
174.00	73688.0
175.00	5479.0
176.00	70472.0
177.00	4960.0
177.90	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
35.90	940.0
37.00	5462.0
38.00	5037.0
38.90	1930.0
39.90	266.0
41.00	228.0
41.90	108.0
42.90	389.0
44.00	1385.0
45.00	977.0
45.90	116.0
47.00	1378.0
47.90	686.0
49.00	4932.0
50.00	22400.0
51.00	6795.0
51.90	359.0
54.90	503.0
55.90	2029.0
57.00	3499.0
57.90	275.0
59.90	1097.0
61.00	5206.0
62.00	5512.0
63.00	4492.0
64.00	356.0
67.00	411.0
68.00	12216.0
69.00	12342.0
70.00	988.0
70.90	145.0
71.20	155.0
72.00	628.0
73.00	4979.0
74.00	19616.0
75.00	59032.0
76.00	5029.0
77.00	677.0
77.90	453.0
78.90	3949.0
79.90	1040.0
80.90	3991.0
81.90	998.0
82.90	198.0
86.10	128.0
87.00	4269.0
87.90	4282.0
90.90	416.0
92.00	3133.0
93.00	4532.0
94.00	12790.0
95.00	109416.0
96.00	7208.0
97.00	232.0
103.80	487.0
104.80	183.0
105.90	540.0
106.90	122.0
110.00	108.0
111.90	112.0
114.90	116.0
115.80	366.0
116.90	750.0
117.90	481.0
118.90	542.0
123.90	113.0
127.80	401.0
128.80	157.0
129.90	395.0
130.90	167.0
134.80	145.0
136.90	145.0
140.90	1065.0
141.80	146.0
142.90	1096.0
145.00	104.0
146.00	132.0
147.90	300.0
152.00	113.0
154.90	221.0
156.90	158.0
159.00	173.0
161.00	119.0
173.10	617.0
174.00	75320.0
175.00	5596.0
176.00	73080.0
177.00	4842.0
177.90	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
35.90	909.0
37.00	5046.0
38.00	4474.0
38.90	1790.0
39.90	225.0
41.00	222.0
42.00	103.0
42.90	390.0
44.00	1322.0
45.00	935.0
45.90	135.0
47.00	1252.0
47.90	654.0
49.00	4279.0
50.00	20392.0
51.00	6280.0
51.90	288.0
54.90	432.0
56.00	1884.0
57.00	3173.0
57.90	249.0
59.90	1070.0
61.00	4798.0
62.00	5097.0
63.00	4061.0
64.00	299.0
66.90	375.0
68.00	10848.0
69.00	11277.0
70.00	923.0
70.90	140.0
71.90	547.0
73.00	4521.0
74.00	17624.0
75.00	54352.0
76.00	4552.0
77.00	561.0
77.90	423.0
78.90	3575.0
79.90	968.0
80.90	3570.0
81.90	963.0
82.90	173.0
87.00	3793.0
87.90	4048.0
90.90	377.0
92.00	2819.0
93.00	4176.0
94.00	11725.0
95.00	101072.0
96.00	6680.0
96.90	225.0
103.90	494.0
104.80	179.0
105.90	490.0
110.90	103.0
114.90	127.0
115.80	343.0
116.90	733.0
117.80	484.0
118.90	527.0
127.80	364.0
128.80	144.0
129.90	359.0
130.80	144.0
134.80	125.0
137.00	135.0
140.90	1026.0
141.80	128.0
142.90	997.0
146.00	121.0
147.90	269.0
154.90	183.0
156.90	127.0
158.90	157.0
173.00	547.0
174.00	70704.0
175.00	5226.0
176.00	69400.0
177.00	4298.0
178.00	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009