

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100318\
 Data File : VU027358.D
 Acq On : 03 Oct 2018 12:12
 Operator : MD/SY
 Sample : VU1003WBL02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1003WBL02

Quant Time: Oct 03 14:42:21 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U100318DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Oct 03 09:31:21 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	5.74	96	22023	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.31	95	5865	0.70	ug/l	0.00
Spiked Amount 1.000			Recovery	=	70.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	5038	0.71	ug/l	0.00
Spiked Amount 1.000			Recovery	=	71.00%	


Target Compounds	Ovalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100318\
Data File : VU027358.D
Acq On : 03 Oct 2018 12:12
Operator : MD/SY
Sample : VU1003WBL02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1003WBL02

Quant Time: Oct 03 14:42:21 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U100318DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Oct 03 09:31:21 2018
Response via : Initial Calibration

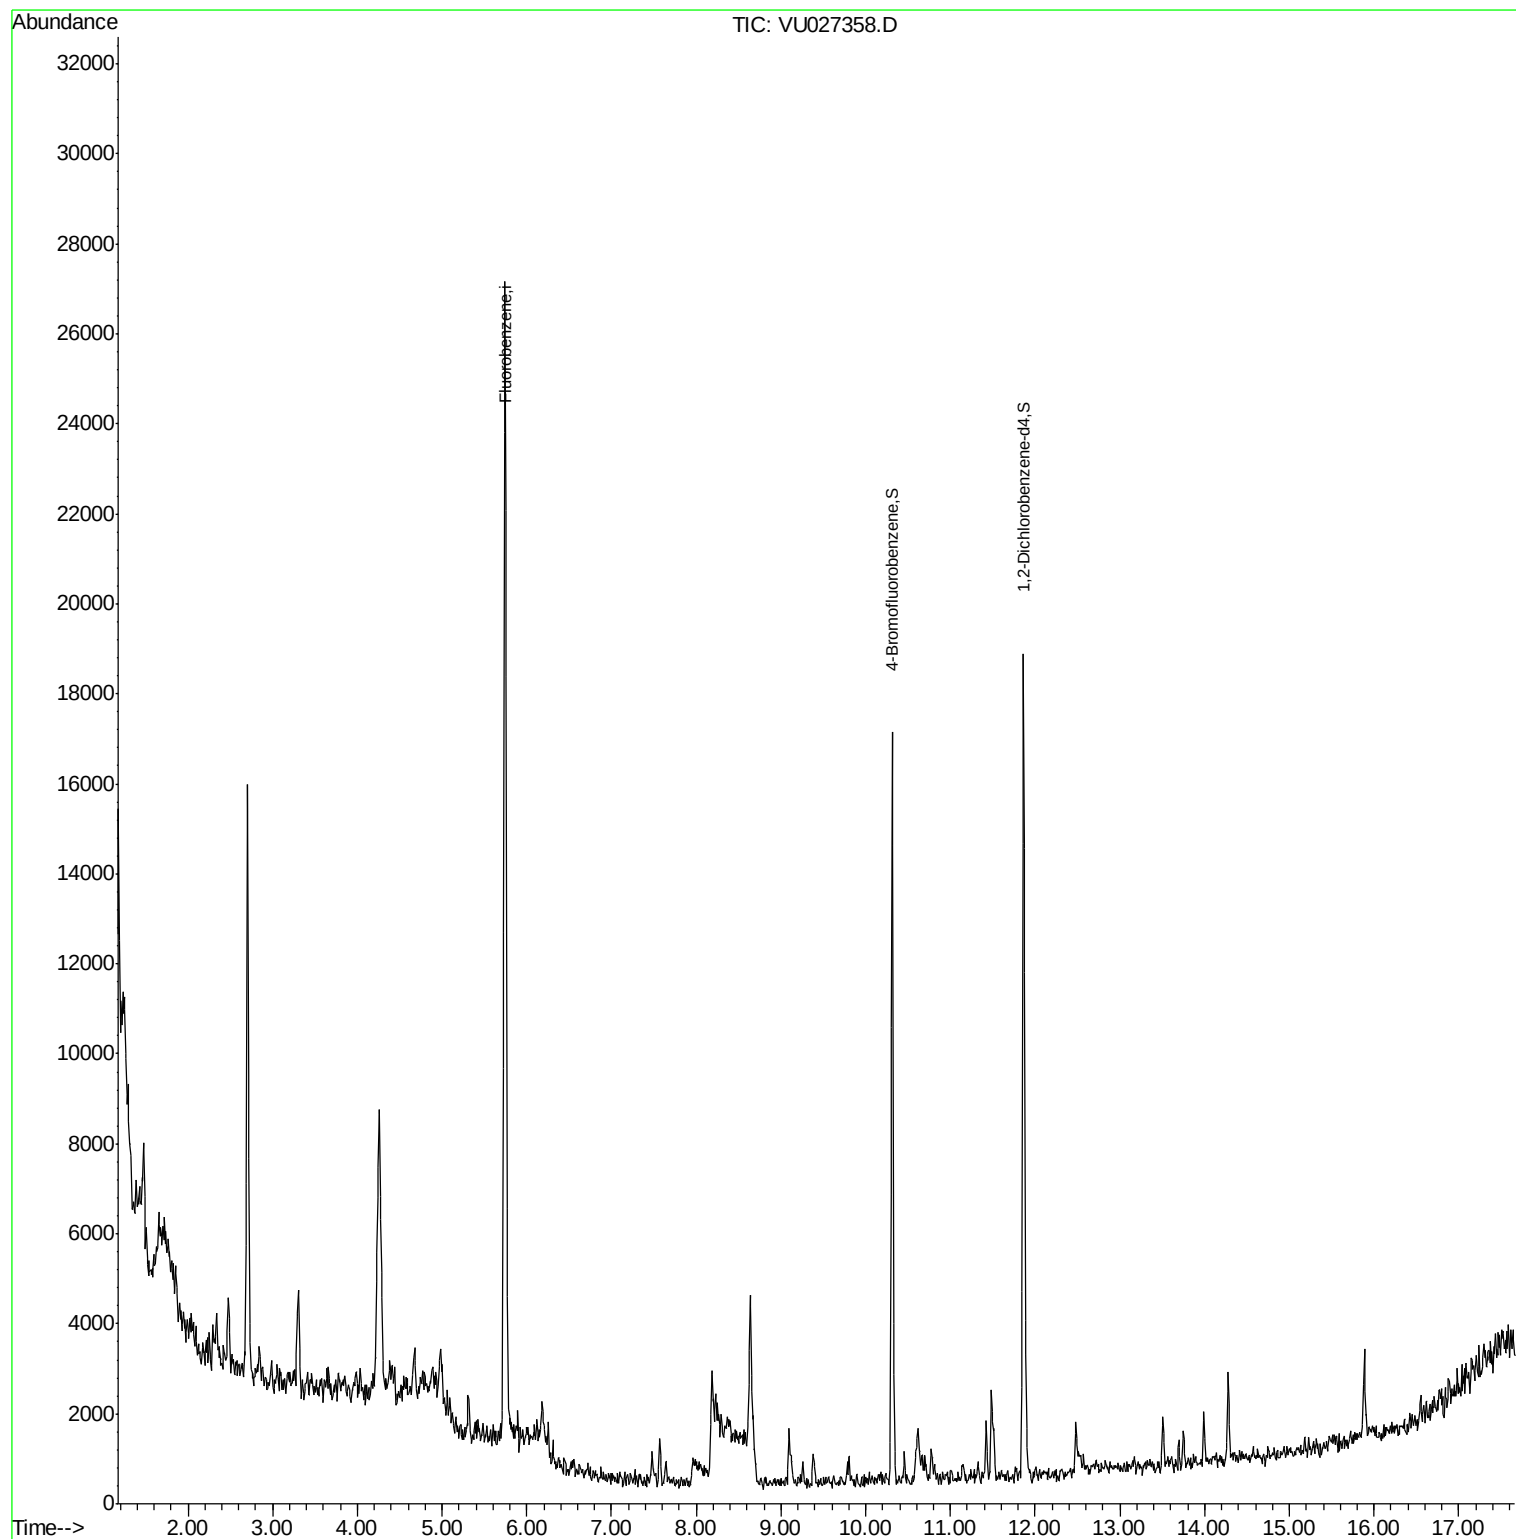

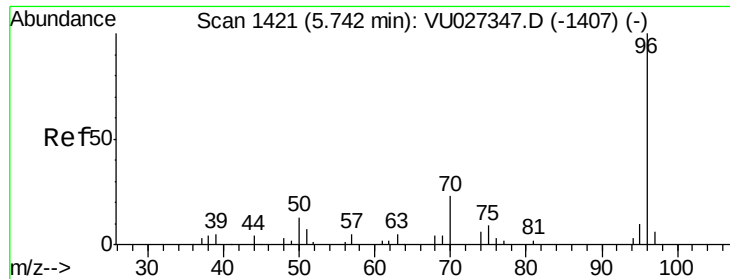

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.74 min Scan# 1421

Delta R.T. 0.00 min

Lab File: VU027358.D

Acq: 03 Oct 2018 12:12

Instrument :

MSVOA_U

ClientSampleId :

VU1003WBL02

Tot Ion: 96 Resp: 22023


Ion Ratio Lower Upper

96 100

70 23.4 19.2 28.8

95 9.8 7.7 11.5

97 6.9 0.0 0.0#



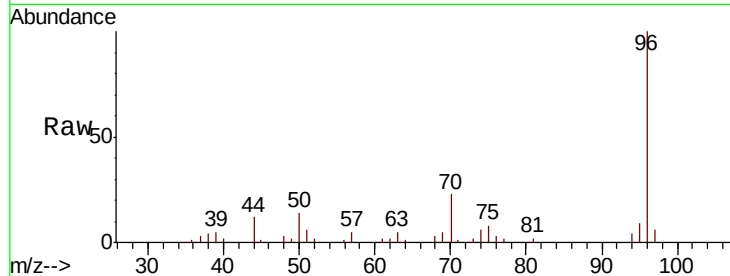


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

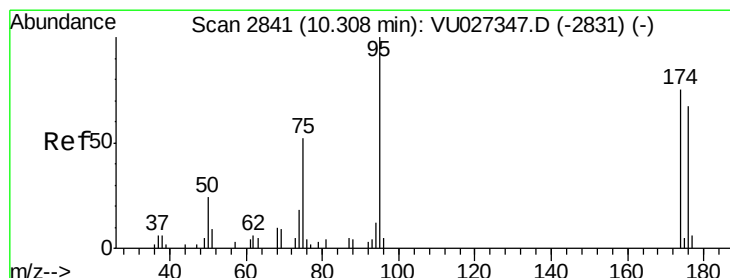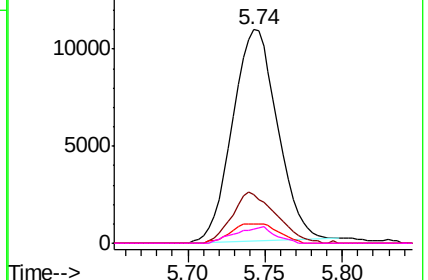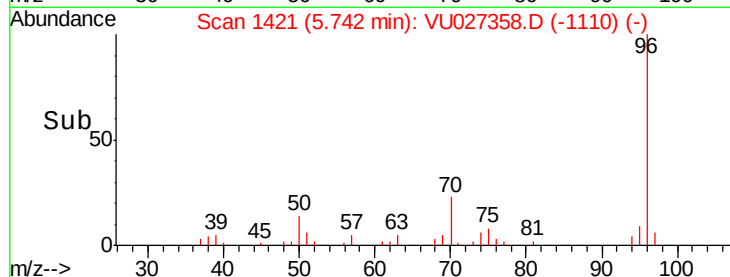

#57

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 10.31 min Scan# 2842

Delta R.T. 0.00 min

Lab File: VU027358.D

Acq: 03 Oct 2018 12:12


Tgt Ion: 95 Resp: 5865

Ion Ratio Lower Upper

95 100

174 75.6 61.0 91.6



176 70.3 57.2 85.8

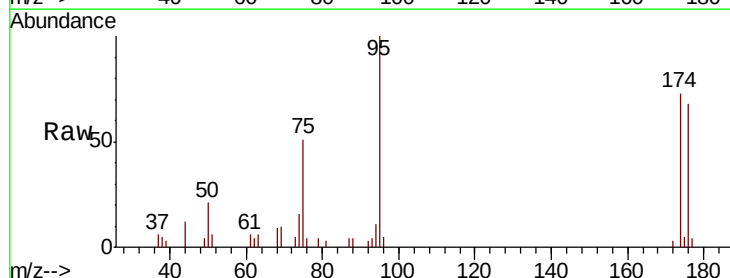


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

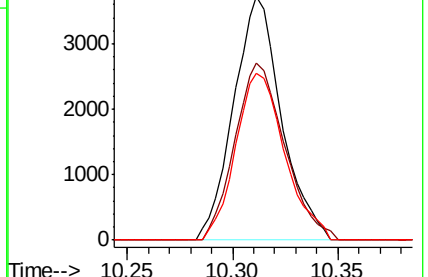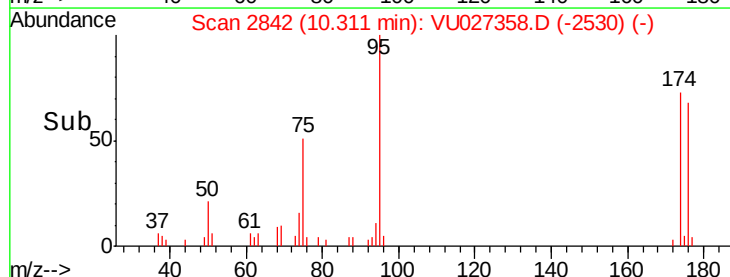


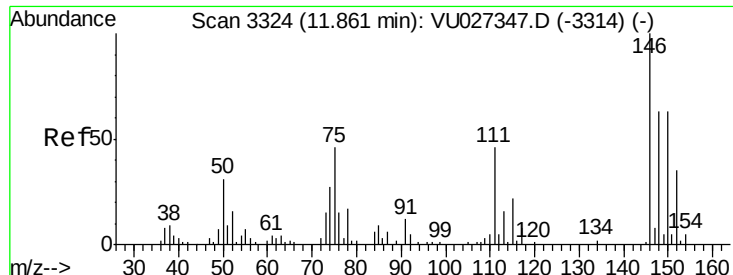

#68
 1,2-Dichlorobenzene-d4
 Concen: N.D. ug/l
 RT: 11.86 min Scan# 3324
 Delta R.T. 0.00 min
 Lab File: VU027358.D
 Acq: 03 Oct 2018 12:12

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1003WBL02

Tot Ion:152 Resp: 5038
 Ion Ratio Lower Upper
 152 100
 115 67.1 0.0 131.6
 150 158.4 0.0 0.0#

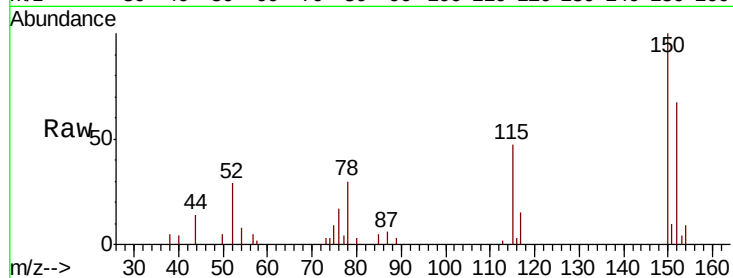

Abundance Ion 152.00 (151.70 to 152.70): V
 Ion 115.00 (114.70 to 115.70): V
 Ion 150.00 (149.70 to 150.70): V

