

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100318\
 Data File : VU027358.D
 Acq On : 03 Oct 2018 12:12
 Operator : MD/SY
 Sample : VU1003WBL02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1003WBL02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U100318DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.292	344	348	351	rBV2	901	900	1.74%	0.445%
2	2.479	399	406	414	rVB4	1663	2883	5.56%	1.425%
3	2.704	467	476	490	rVB	13129	21952	42.35%	10.852%
4	2.839	516	518	526	rVB3	783	931	1.80%	0.460%
5	3.302	653	662	673	rVB7	2420	5301	10.23%	2.621%
6	3.611	755	758	764	rBV3	513	710	1.37%	0.351%
7	3.778	806	810	812	rBV3	638	547	1.06%	0.270%
8	4.260	946	960	976	rVB3	5944	16883	32.57%	8.346%
9	5.742	1408	1421	1435	rBV3	25720	51835	100.00%	25.625%
10	5.922	1473	1477	1481	rBV3	571	547	1.06%	0.270%
11	6.254	1576	1580	1585	rVB3	817	656	1.27%	0.324%
12	7.572	1983	1990	1996	rVB4	1059	1689	3.26%	0.835%
13	7.639	2003	2011	2018	rBV3	491	768	1.48%	0.380%
14	7.964	2099	2112	2116	rBV3	661	1310	2.53%	0.648%
15	8.186	2170	2181	2185	rBV5	2367	4052	7.82%	2.003%
16	8.231	2189	2195	2199	rVV4	682	1028	1.98%	0.508%
17	8.292	2211	2214	2222	rVB6	515	524	1.01%	0.259%
18	8.639	2311	2322	2331	rBV4	3049	5185	10.00%	2.563%
19	9.096	2458	2464	2469	rBV3	1253	1700	3.28%	0.840%
20	9.257	2509	2514	2525	rVB2	517	555	1.07%	0.274%
21	9.379	2546	2552	2558	rBV3	713	1157	2.23%	0.572%
22	10.311	2833	2842	2856	rVB2	16732	26089	50.33%	12.897%
23	10.456	2882	2887	2893	rVB3	701	688	1.33%	0.340%
24	10.617	2919	2937	2945	rBV5	1213	3230	6.23%	1.597%
25	10.774	2979	2986	2992	rBV3	682	944	1.82%	0.467%
26	11.324	3151	3157	3167	rVB2	472	764	1.47%	0.378%
27	11.424	3181	3188	3196	rVB3	1303	1683	3.25%	0.832%
28	11.482	3201	3206	3213	rBV2	1832	2555	4.93%	1.263%
29	11.861	3315	3324	3342	rBV2	18317	32409	62.52%	16.022%
30	12.482	3510	3517	3524	rBV3	1123	1757	3.39%	0.869%
31	13.504	3830	3835	3836	rBV	978	712	1.37%	0.352%
32	13.752	3903	3912	3917	rBV	887	1266	2.44%	0.626%
33	13.990	3980	3986	3994	rBV2	1219	1536	2.96%	0.759%
34	14.279	4067	4076	4084	rBV2	1962	2954	5.70%	1.460%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100318\
Data File : VU027358.D
Acq On : 03 Oct 2018 12:12
Operator : MD/SY
Sample : VU1003WBL02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1003WBL02

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U100318DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

35	15.883	4567	4575	4581	rBV3	1739	2236	4.31%	1.105%
36	16.842	4870	4873	4879	rBV5	643	694	1.34%	0.343%
37	17.031	4928	4932	4935	rBV3	684	526	1.01%	0.260%
38	17.083	4946	4948	4952	rBV4	670	546	1.05%	0.270%
39	17.613	5109	5113	5116	rBV4	619	582	1.12%	0.288%


Sum of corrected areas: 202284

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100318\
Data File : VU027358.D
Acq On : 03 Oct 2018 12:12
Operator : MD/SY
Sample : VU1003WBL02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1003WBL02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U100318DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

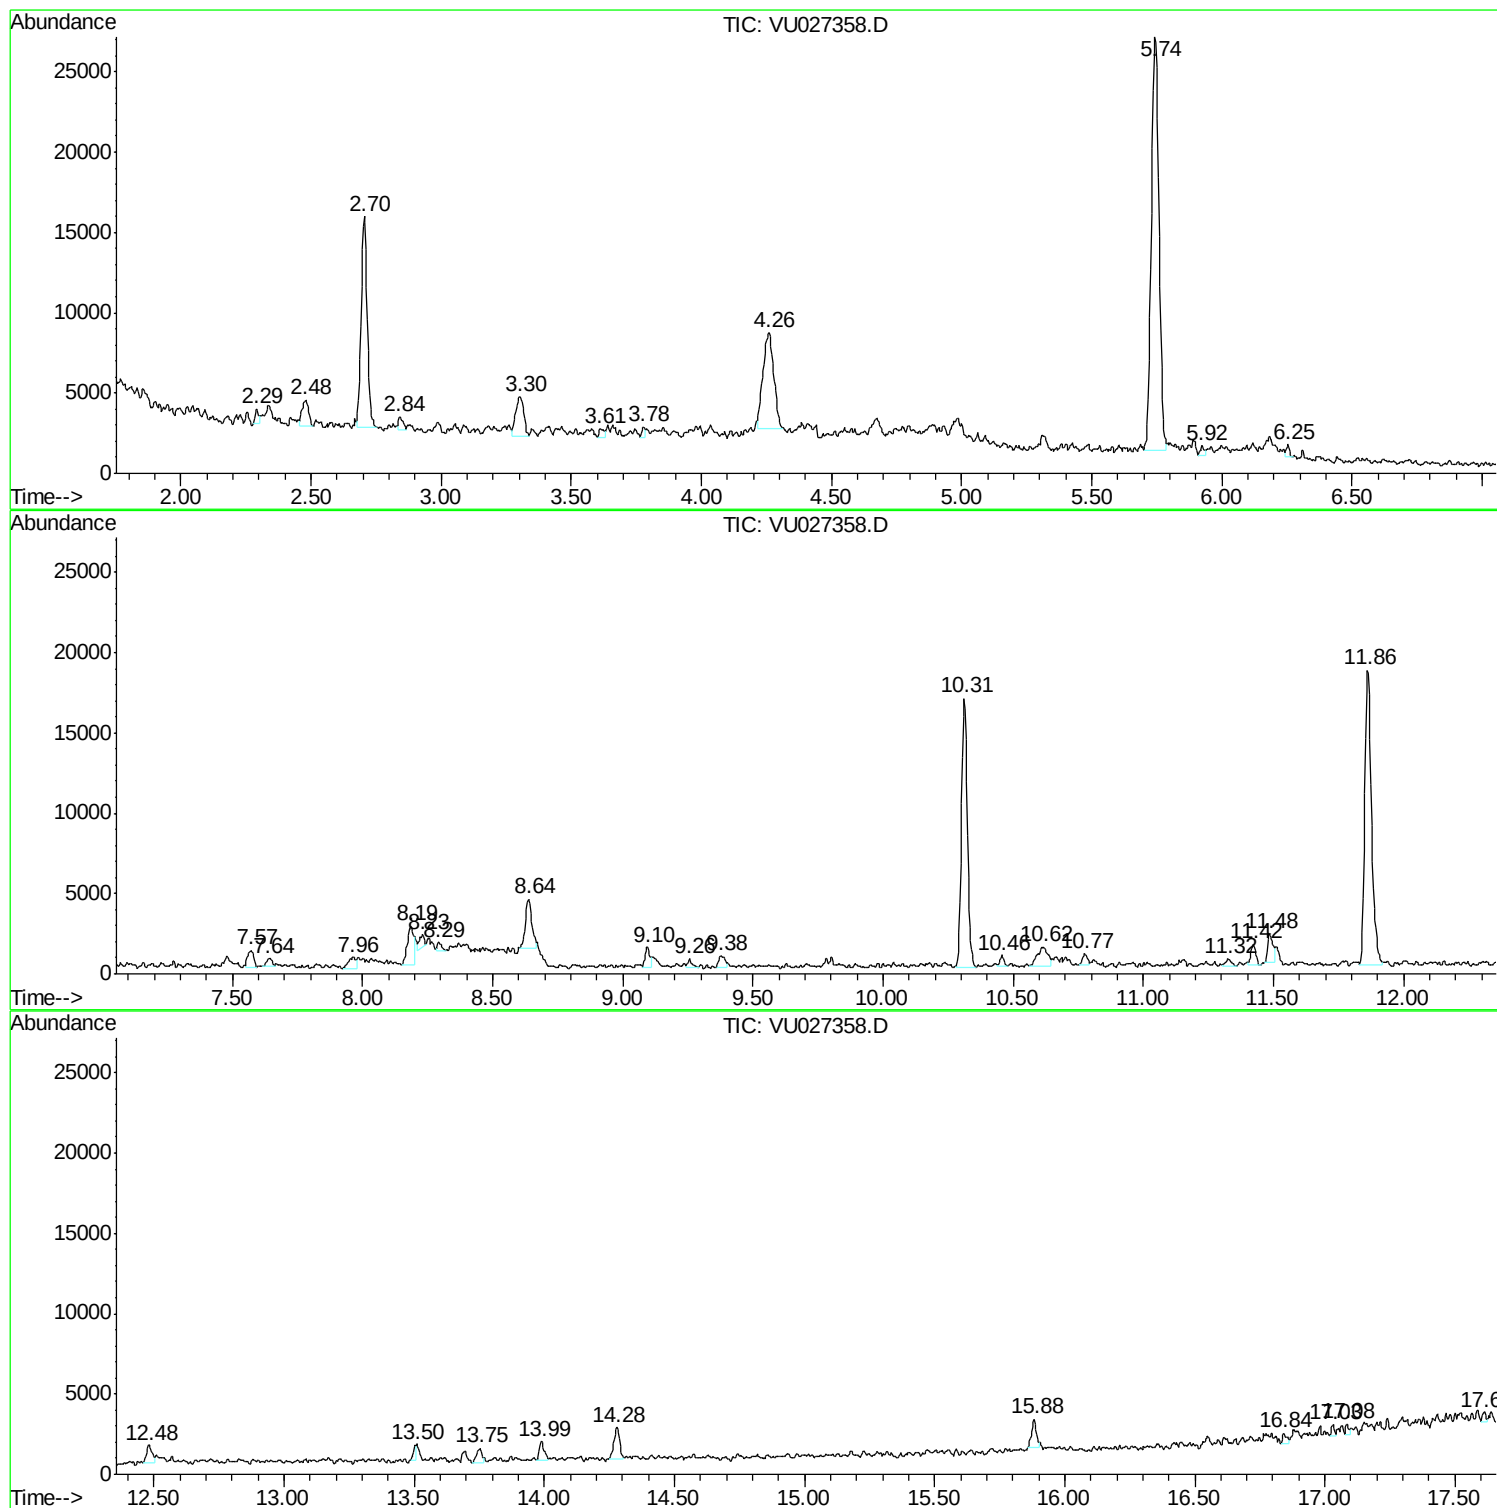

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU100318\
Data File : VU027358.D
Acq On : 03 Oct 2018 12:12
Operator : MD/SY
Sample : VU1003WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1003WBL02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U100318DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU100318\
Data File : VU027358.D
Acq On : 03 Oct 2018 12:12
Operator : MD/SY
Sample : VU1003WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1003WBL02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U100318DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc