


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100318\
Data File : VU027342.D
Acq On : 02 Oct 2018 14:15
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U100318DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Wed Oct 03 17:14:05 2018

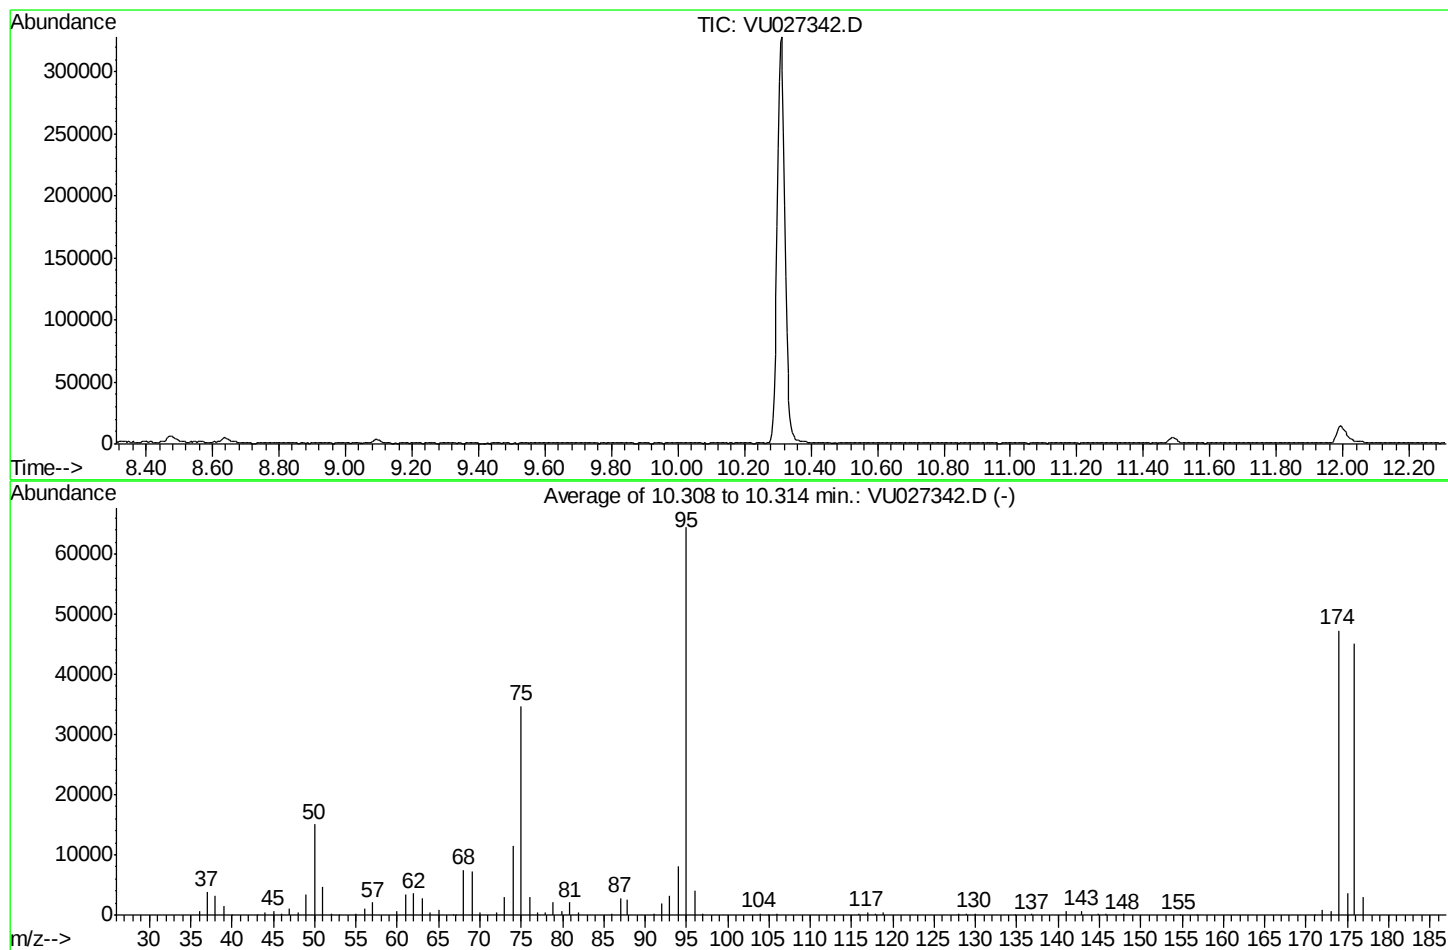

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	15064	PASS
75	95	30	60	53.9	34714	PASS
95	95	100	100	100.0	64434	PASS
96	95	5	9	6.4	4155	PASS
173	174	0.00	2	1.3	608	PASS
174	95	50	100	73.4	47288	PASS
175	174	5	9	7.7	3637	PASS
176	174	95	101	95.3	45042	PASS
177	176	5	9	6.6	2959	PASS