


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100318\
Data File : VU027356.D
Acq On : 03 Oct 2018 10:44
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U100318DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Wed Oct 03 17:14:05 2018

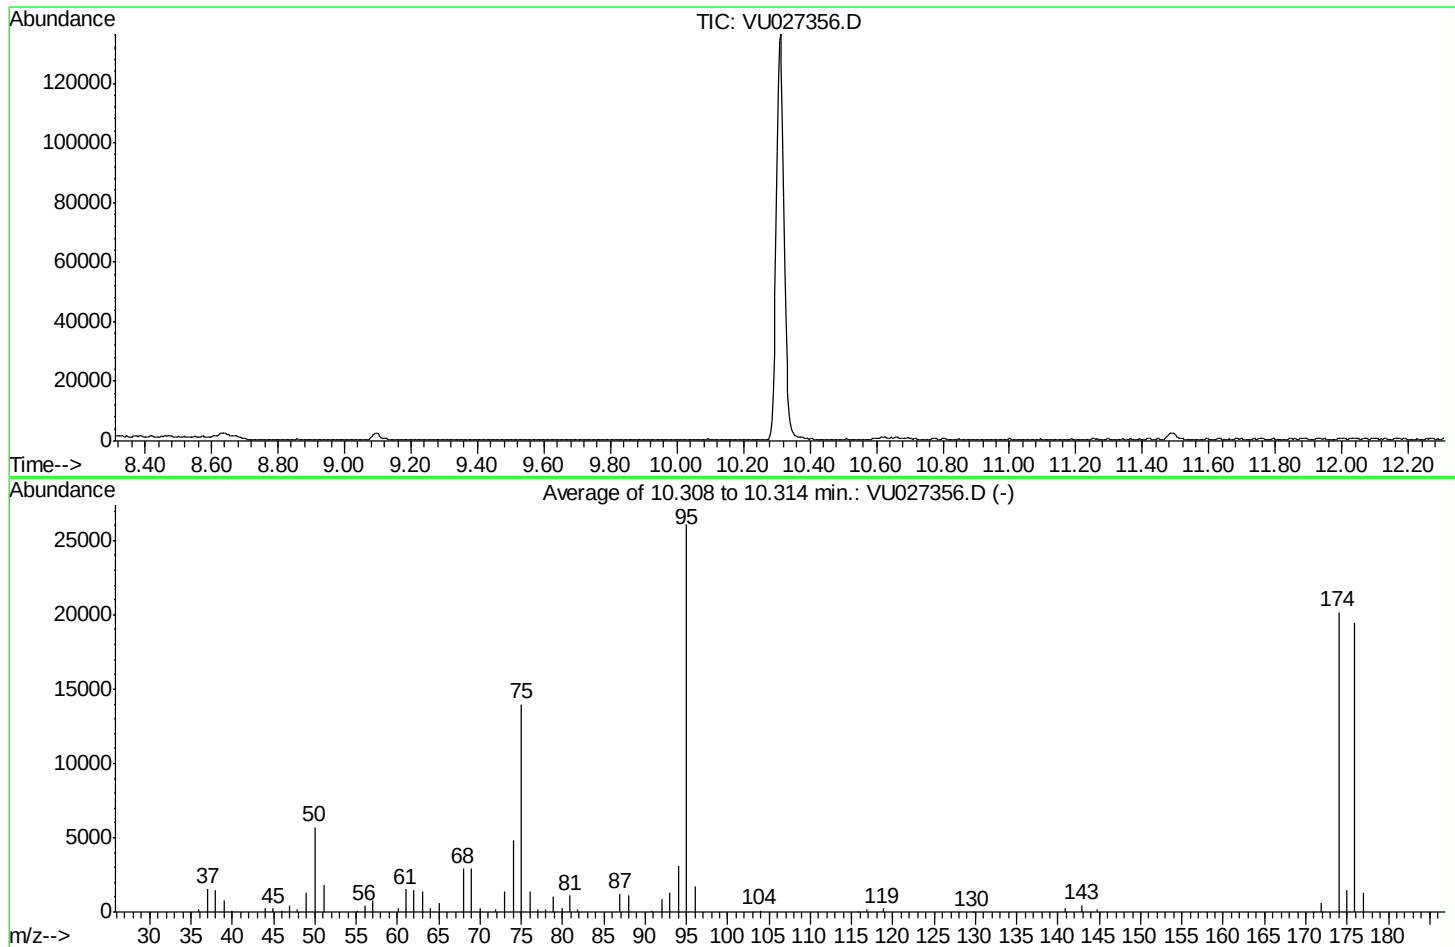

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	5728	PASS
75	95	30	60	53.5	13956	PASS
95	95	100	100	100.0	26090	PASS
96	95	5	9	6.7	1755	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.3	20170	PASS
175	174	5	9	7.2	1455	PASS
176	174	95	101	96.4	19448	PASS
177	176	5	9	6.8	1322	PASS