


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100319\
 Data File : VU034910.D
 Acq On : 03 Oct 2019 08:56
 Operator : JC/SP
 Sample : BFB42
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100319WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 04 07:30:57 2019

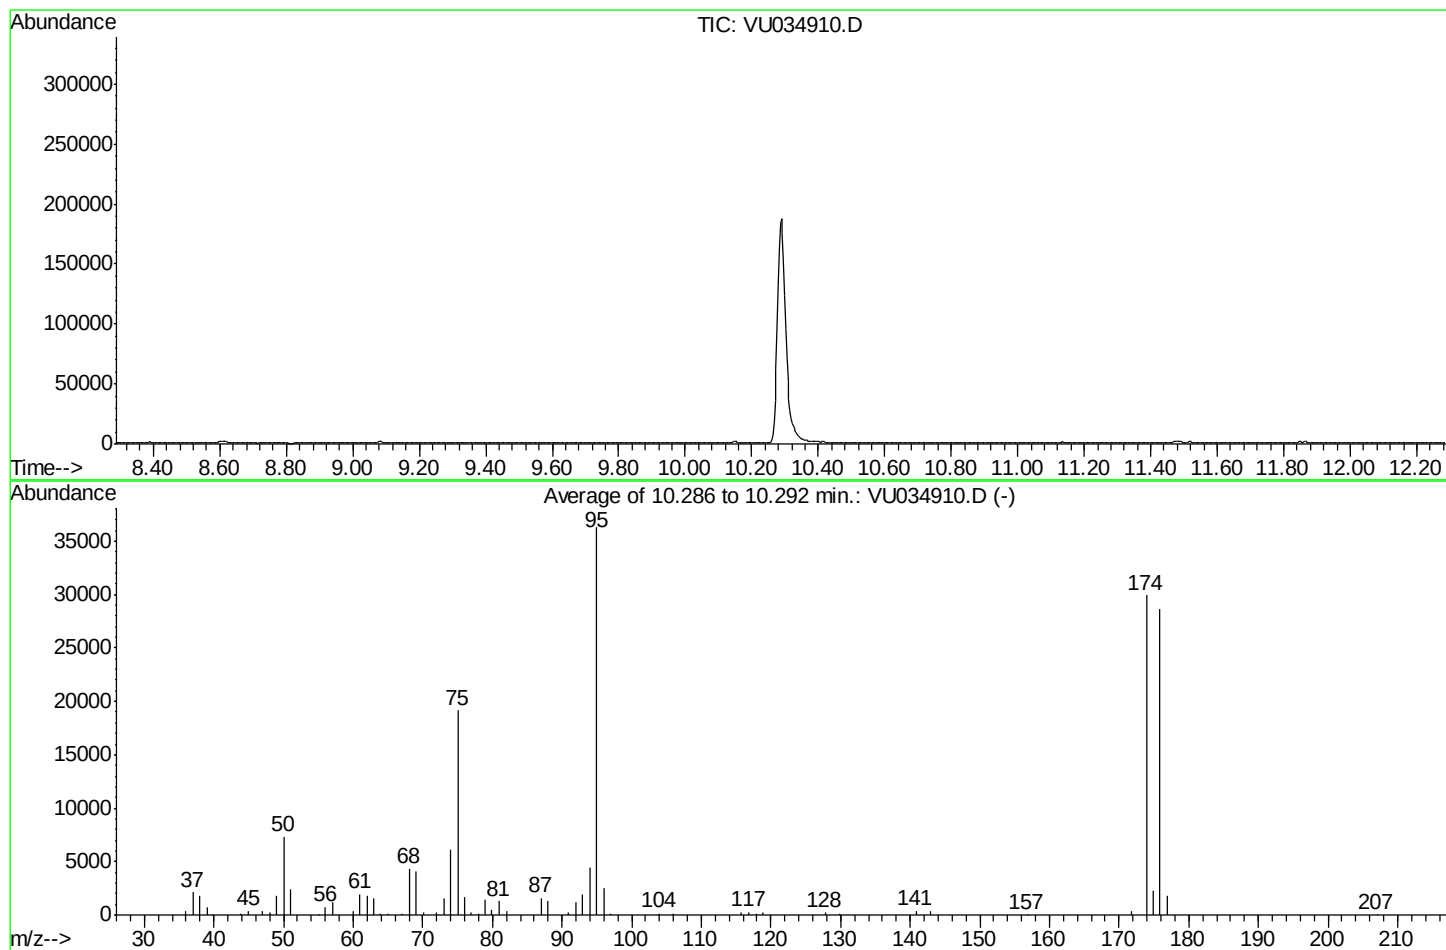

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	7313	PASS
75	95	30	80	52.8	19157	PASS
95	95	100	100	100.0	36293	PASS
96	95	5	9	7.0	2548	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.5	29941	PASS
175	174	5	9	7.8	2332	PASS
176	174	95	101	95.6	28621	PASS
177	176	5	9	6.2	1788	PASS

m/z	Abundance
36.00	378.0
37.00	2184.0
38.00	1857.0
39.00	661.0
39.80	167.0
44.00	667.0
45.00	423.0
47.00	391.0
48.10	191.0
49.00	1729.0
50.00	7763.0
51.00	2476.0
55.00	111.0
56.00	673.0
57.00	1237.0
60.00	399.0
61.00	1865.0
62.00	1883.0
63.00	1617.0
63.90	241.0
65.00	102.0
66.90	133.0
68.00	4370.0
69.00	3972.0
70.10	321.0
71.90	216.0
73.00	1553.0
74.00	6346.0
75.00	19568.0
76.00	1701.0
76.90	241.0
78.00	202.0
78.90	1456.0
79.90	523.0
80.90	1382.0
82.00	308.0
86.90	1615.0
87.90	1437.0
90.80	182.0
92.00	1251.0
93.00	1900.0
94.00	4437.0
95.00	37320.0
96.00	2597.0
96.90	109.0
103.90	156.0
105.90	187.0
115.80	195.0
116.90	260.0
117.90	127.0
118.90	201.0
127.80	156.0
129.80	224.0
140.80	367.0
142.90	367.0
171.80	344.0
173.90	29488.0
174.90	2416.0
175.90	27712.0
176.90	1701.0
207.00	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	404.0
37.00	2171.0
38.00	1863.0
39.00	717.0
40.00	197.0
44.00	665.0
45.00	406.0
47.00	380.0
48.10	199.0
49.00	1823.0
50.00	7507.0
51.00	2530.0
56.00	754.0
57.00	1247.0
59.90	414.0
61.00	1962.0
62.00	1874.0
63.00	1595.0
63.90	158.0
65.00	104.0
66.90	106.0
68.00	4483.0
69.00	4166.0
70.10	282.0
71.90	197.0
73.00	1524.0
74.00	6288.0
75.00	19656.0
76.00	1707.0
76.90	219.0
78.00	175.0
78.90	1502.0
79.90	520.0
80.90	1346.0
82.00	338.0
87.00	1646.0
87.90	1350.0
90.90	197.0
92.00	1268.0
93.00	1970.0
94.00	4638.0
95.00	37352.0
96.00	2629.0
96.90	102.0
104.00	183.0
105.90	160.0
115.80	196.0
116.90	289.0
117.90	106.0
118.80	217.0
127.80	201.0
129.80	167.0
140.80	415.0
142.90	395.0
156.80	107.0
171.90	324.0
173.90	30824.0
174.90	2427.0
175.90	29648.0
176.90	1841.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	398.0
37.00	2008.0
38.00	1676.0
39.00	738.0
40.00	262.0
43.90	696.0
45.00	343.0
46.90	397.0
48.10	221.0
49.00	1690.0
50.00	6669.0
51.00	2314.0
56.00	741.0
57.00	1157.0
59.90	392.0
61.00	1932.0
62.00	1713.0
63.00	1428.0
65.10	125.0
68.00	4125.0
69.00	3975.0
70.10	230.0
71.90	191.0
73.00	1509.0
74.00	5851.0
75.00	18248.0
76.10	1560.0
77.00	233.0
78.00	151.0
78.90	1450.0
79.90	441.0
80.90	1221.0
82.00	356.0
87.00	1519.0
87.90	1254.0
91.00	207.0
91.90	1128.0
93.00	1799.0
94.00	4360.0
95.00	34208.0
96.00	2420.0
104.00	199.0
105.90	120.0
115.70	180.0
116.80	273.0
118.80	214.0
127.80	214.0
129.70	116.0
140.80	438.0
142.90	379.0
171.90	275.0
173.90	29512.0
174.90	2153.0
175.90	28504.0
176.90	1823.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

Scan 2849 (10.251 min): VU034910.D
BFB42

m/z	Abundance
40.00	240.0
41.10	107.0
43.90	603.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42