

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100320\
 Data File : VU040478.D
 Acq On : 03 Oct 2020 14:42
 Operator : SY/MD
 Sample : VU1003WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK22

Quant Time: Oct 05 01:09:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 05 00:56:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	129216	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	129788	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	55996	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	34187	5.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.80%
7) Chloroethane-d5	1.93	69	29104	5.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.00%
11) 1,1-Dichloroethene-d2	2.58	63	54295	3.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.60%
20) 2-Butanone-d5	4.66	46	137141	43.16	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.32%
24) Chloroform-d	5.08	84	71295	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
26) 1,2-Dichloroethane-d4	5.72	65	44041	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
32) Benzene-d6	5.74	84	137068	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.00%
36) 1,2-Dichloropropane-d6	6.70	67	46561	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	7.91	98	114000	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
43) trans-1,3-Dichloropropene-	8.19	79	18828	4.83	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.60%
46) 2-Hexanone-d5	8.64	63	93271	40.71	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.42%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	41211	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.80%
64) 1,2-Dichlorobenzene-d4	12.19	152	43658	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%


Target Compounds					Ovalue
16) Methylene chloride	3.06	84	2621	0.212 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100320\
Data File : VU040478.D
Acq On : 03 Oct 2020 14:42
Operator : SY/MD
Sample : VU1003WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK22

Quant Time: Oct 05 01:09:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 05 00:56:13 2020
Response via : Initial Calibration

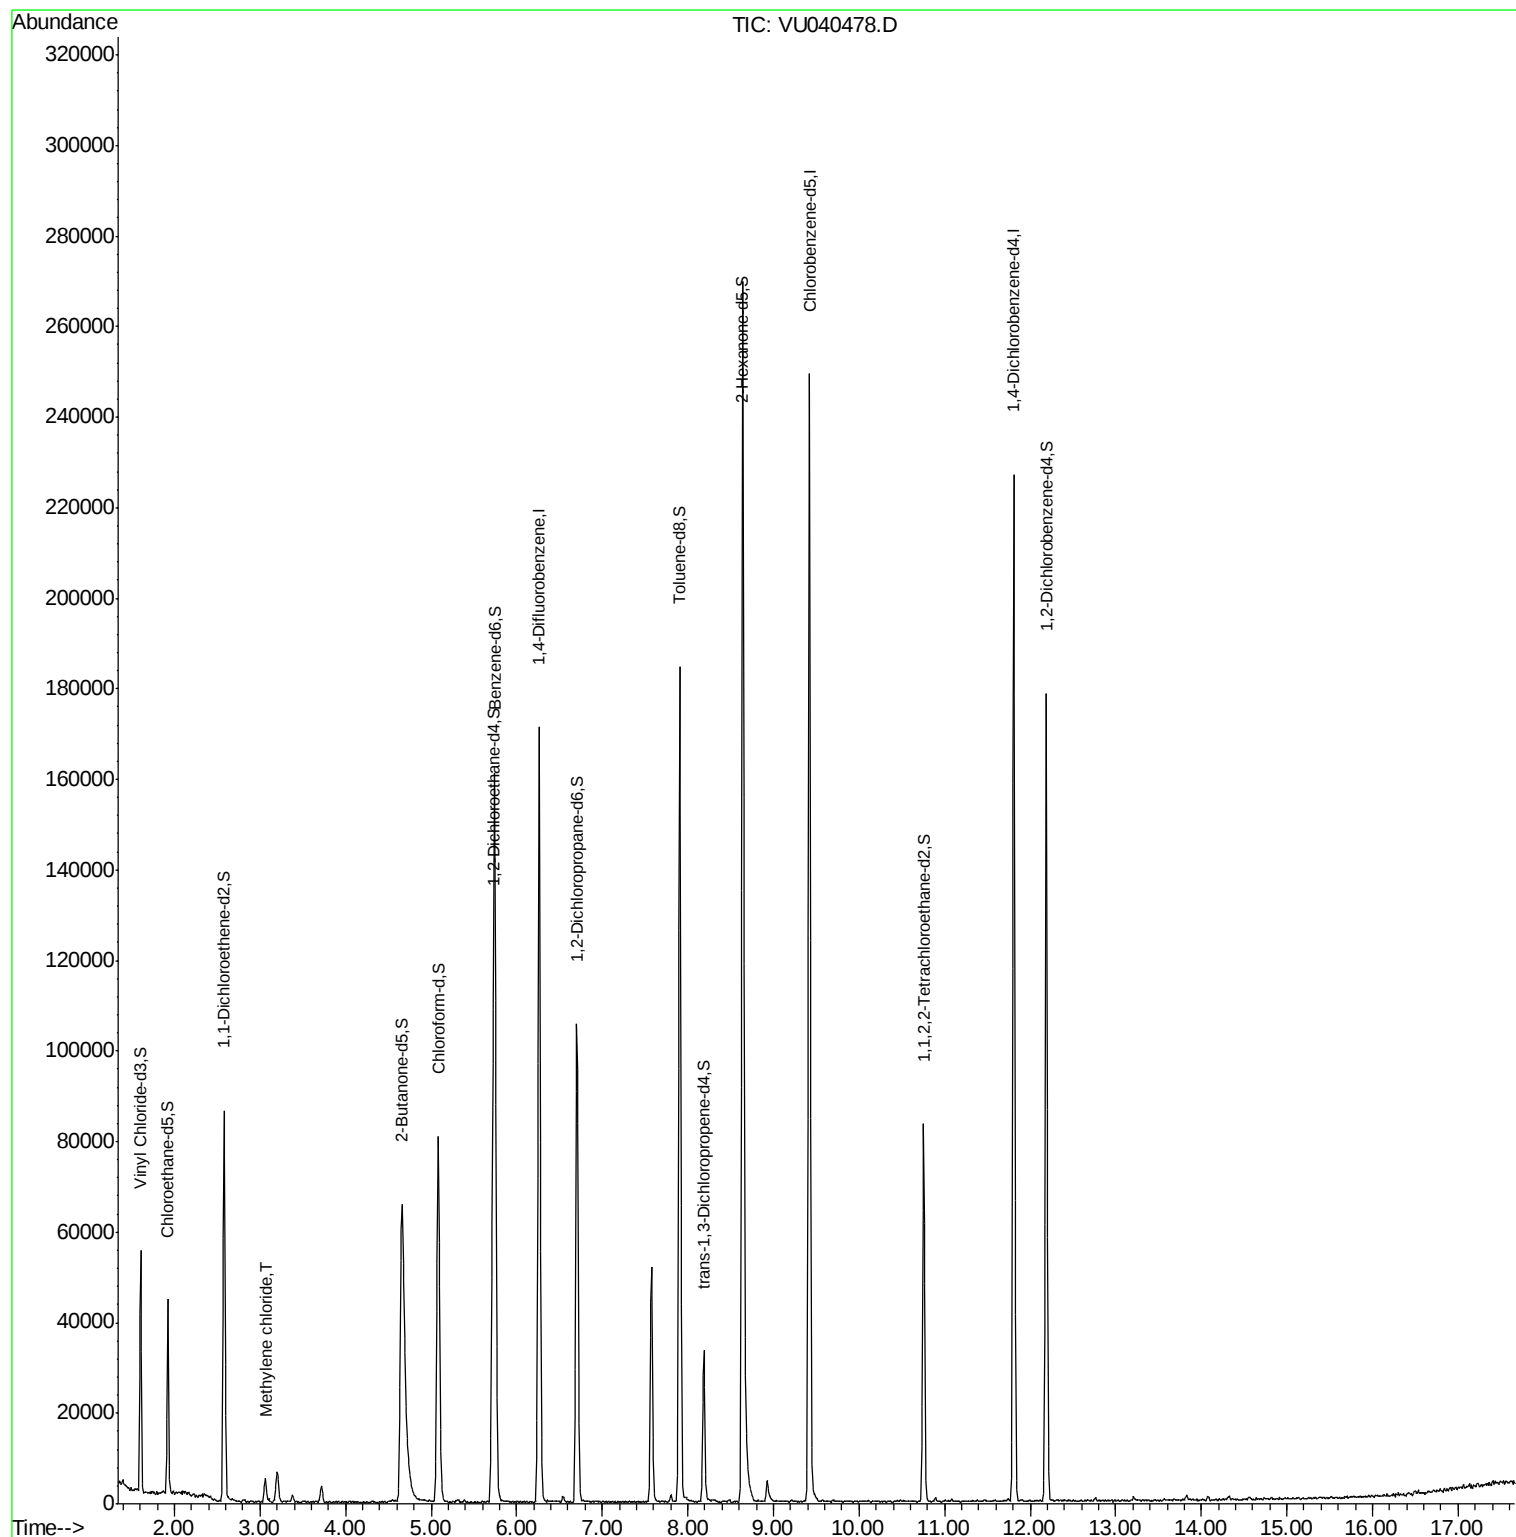

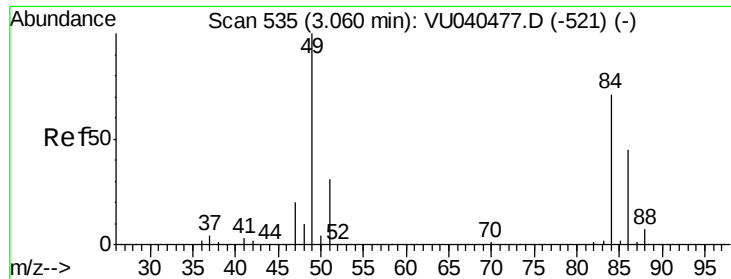

#16
 Methvlene chloride
 Concen: 0.212 ug/L
 RT: 3.06 min Scan# 535
 Delta R.T. -0.00 min
 Lab File: VU040478.D
 Acq: 03 Oct 2020 14:42

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK22

Tot Ion:	84	Resp:	2621
Ion	Ratio	Lower	Upper
84	100		
86	54.7	44.4	82.5
49	117.9	92.2	171.2

