

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U100320\
 Data File : VU040479.D
 Acq On : 03 Oct 2020 15:09
 Operator : SY/MD
 Sample : L4266-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFZR3

Quant Time: Oct 05 01:13:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 05 00:56:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	122753	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	123074	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	52908	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	31392	5.17	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.40%
7) Chloroethane-d5	1.92	69	27205	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.20%
11) 1,1-Dichloroethene-d2	2.58	63	51462	3.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.40%
20) 2-Butanone-d5	4.66	46	130688	43.29	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.58%
24) Chloroform-d	5.08	84	69204	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
26) 1,2-Dichloroethane-d4	5.72	65	41725	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
32) Benzene-d6	5.74	84	125756	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
36) 1,2-Dichloropropane-d6	6.70	67	43680	4.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.60%
41) Toluene-d8	7.91	98	104285	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
43) trans-1,3-Dichloropropene-	8.19	79	17117	4.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.60%
46) 2-Hexanone-d5	8.64	63	88092	40.55	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.10%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	37107	4.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	42310	5.27	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.40%


Target Compounds					Ovalue
13) Acetone	2.67	43	16683	6.632 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100320\
Data File : VU040479.D
Acq On : 03 Oct 2020 15:09
Operator : SY/MD
Sample : L4266-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFZR3

Quant Time: Oct 05 01:13:20 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 05 00:56:13 2020
Response via : Initial Calibration

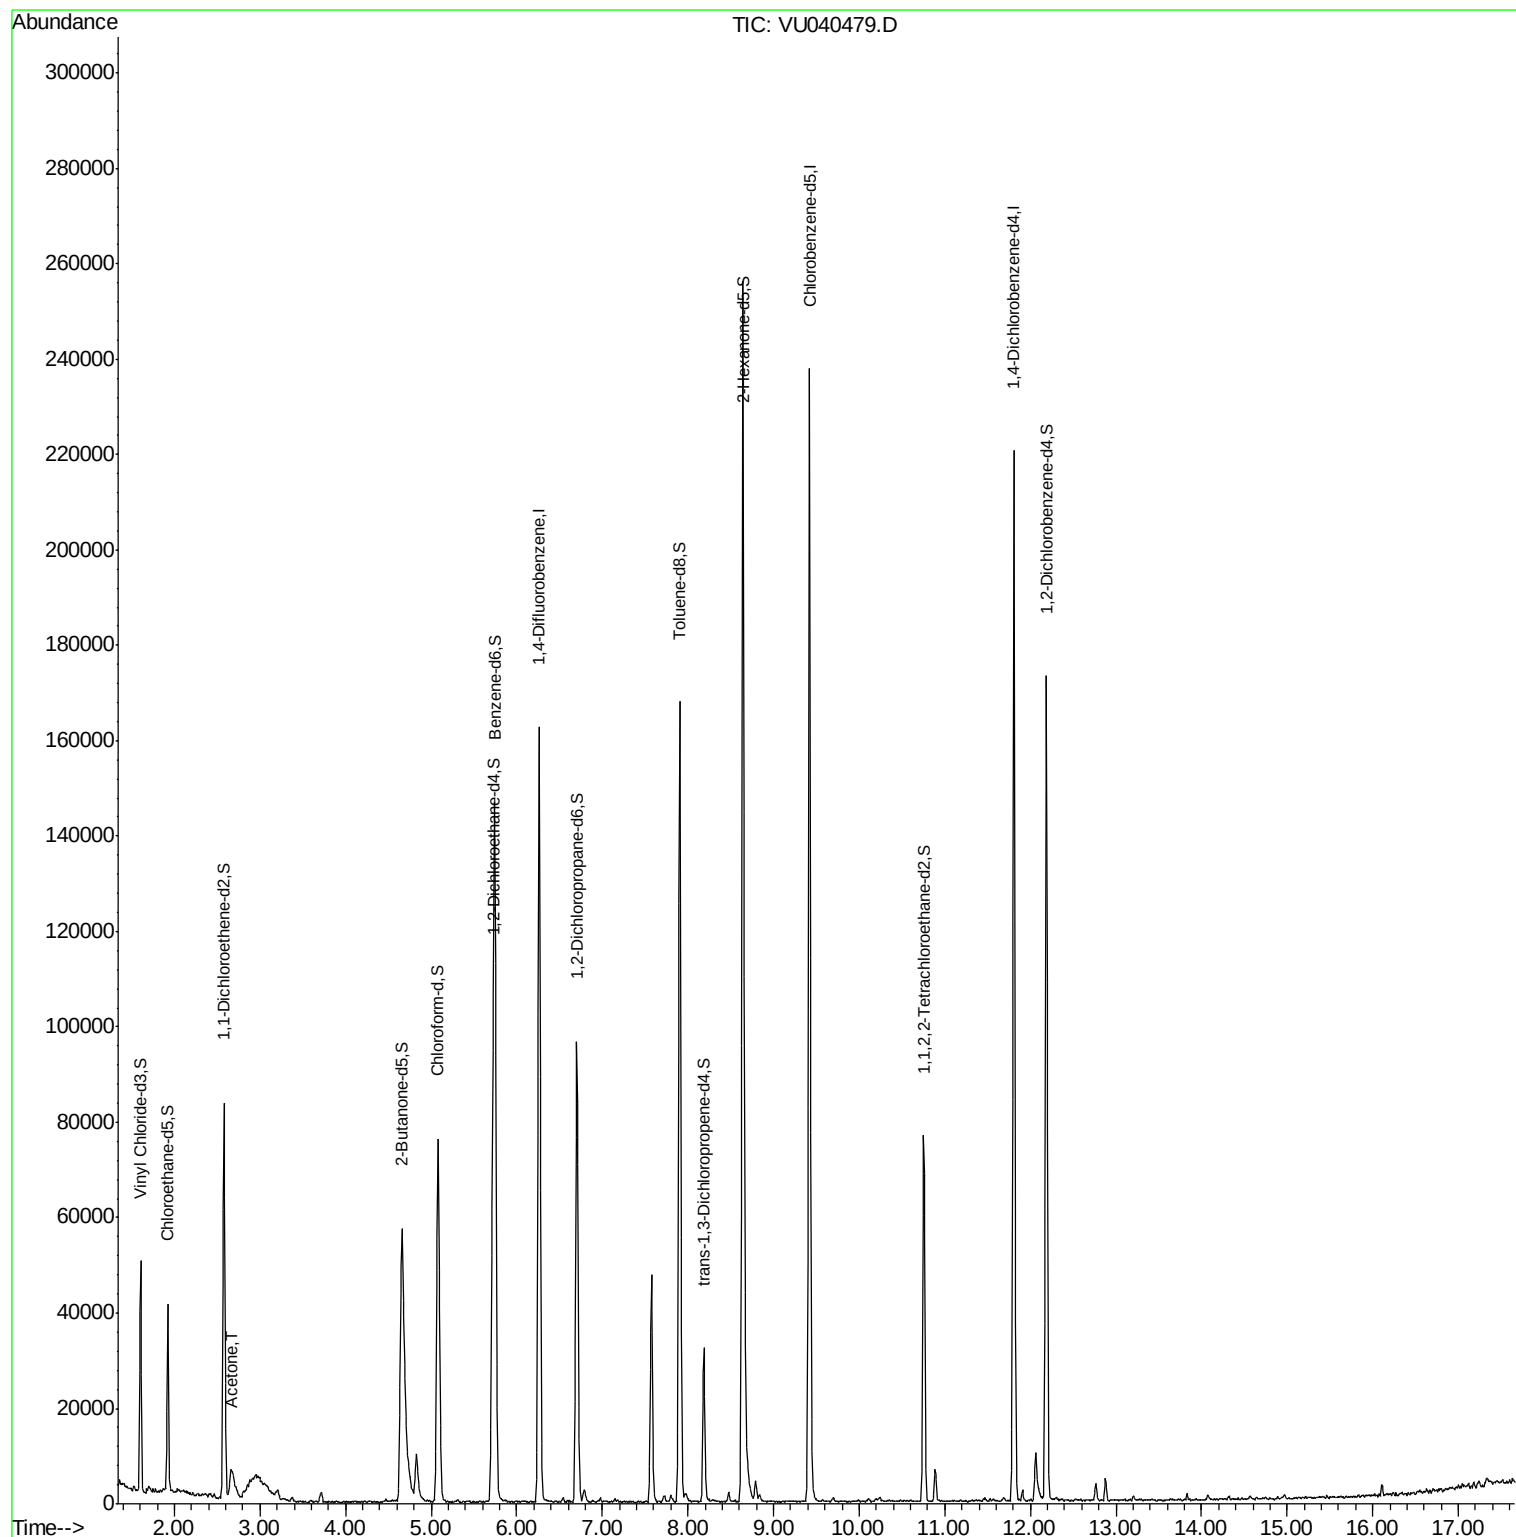

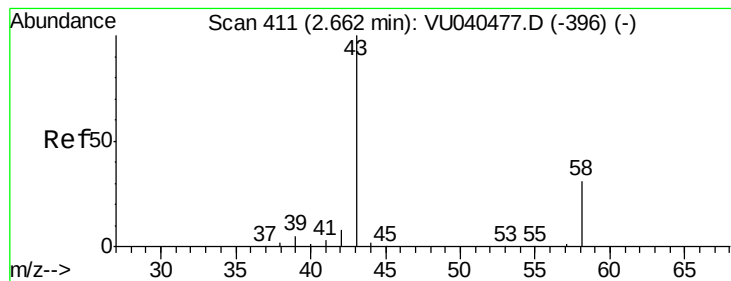

#13

Acetone

Concen: 6.632 ug/L

RT: 2.67 min Scan# 413

Delta R.T. 0.01 min

Lab File: VU040479.D

Acq: 03 Oct 2020 15:09

Instrument :
MSVOA_U
ClientSampleId :
BFZR3

Tot Ion: 43 Resp: 16683

Ion Ratio Lower Upper

43 100

58 22.6 0.0 61.8

