


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100320\
 Data File : VU040476.D
 Acq On : 03 Oct 2020 12:39
 Operator : SY/MD
 Sample : BFB13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB13

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Oct 05 00:56:13 2020

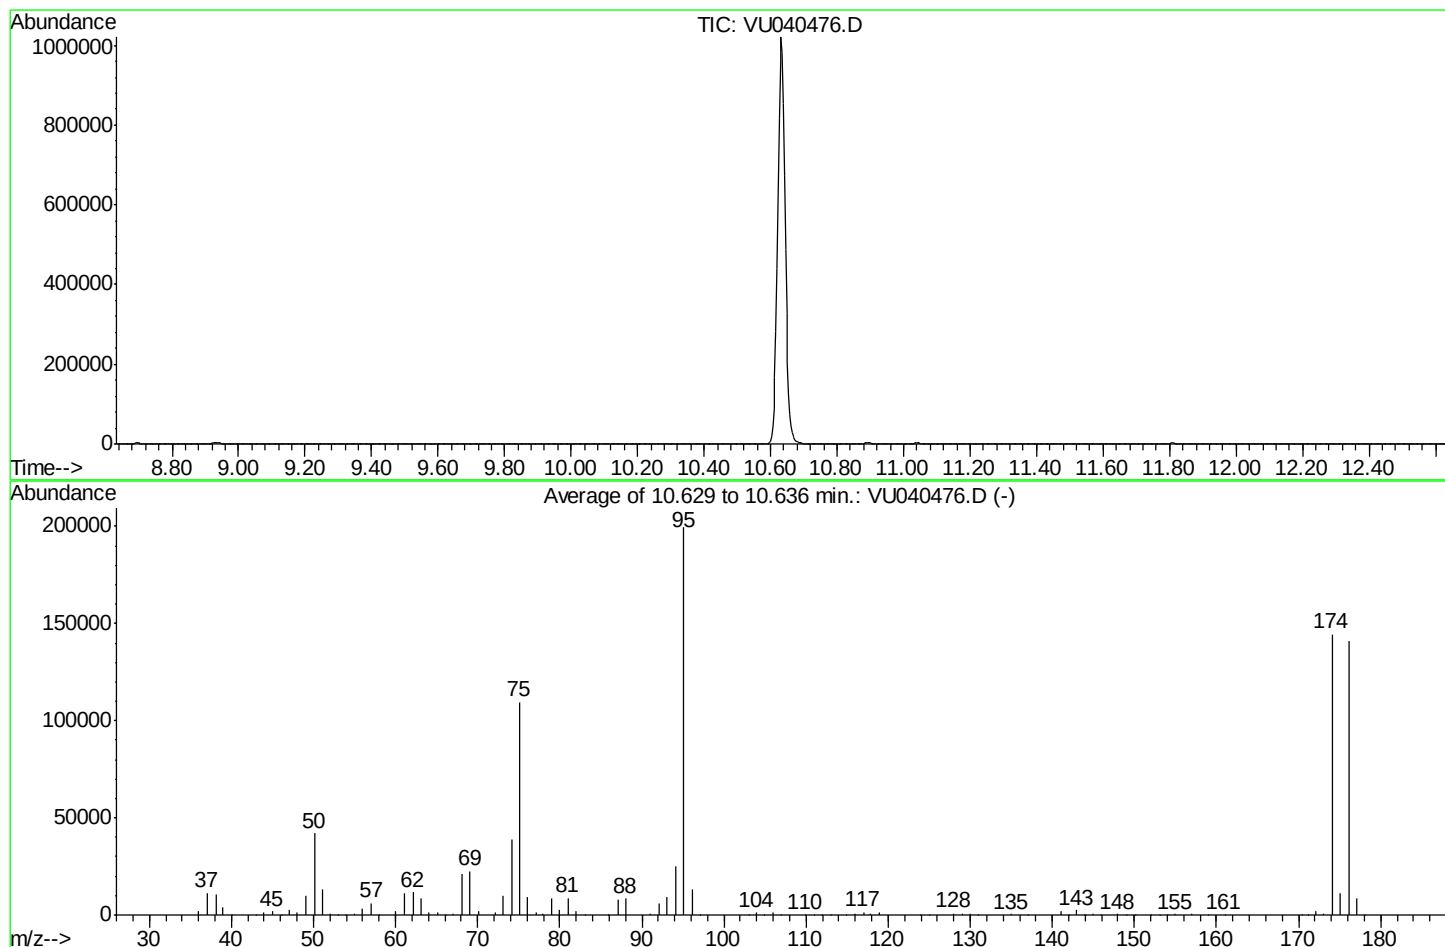

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	41930	PASS
75	95	30	80	54.8	109426	PASS
95	95	100	100	100.0	199509	PASS
96	95	5	9	6.7	13309	PASS
173	174	0.00	2	0.5	711	PASS
174	95	50	120	72.4	144469	PASS
175	174	5	9	7.8	11259	PASS
176	174	95	101	97.4	140714	PASS
177	176	5	9	6.2	8695	PASS

m/z	Abundance
36.00	2249.0
37.00	11651.0
38.10	10503.0
39.00	4156.0
40.00	322.0
44.00	1715.0
45.00	1865.0
46.10	315.0
47.00	2732.0
48.00	1305.0
49.10	9946.0
50.10	41312.0
51.10	13132.0
52.00	637.0
53.00	176.0
55.00	565.0
56.00	3447.0
57.00	5949.0
58.00	176.0
60.10	1878.0
61.10	11036.0
62.10	11305.0
63.10	9071.0
64.10	1256.0
65.10	1445.0
66.00	207.0
67.00	604.0
68.10	20904.0
69.10	22648.0
70.10	1971.0
72.10	1176.0
73.10	9877.0
74.10	38168.0
75.10	107720.0
76.10	8961.0
77.10	1221.0
77.90	851.0
79.00	8388.0
80.00	2751.0
81.00	8596.0
82.00	2132.0
83.00	169.0
85.90	289.0
87.00	7554.0
88.00	8179.0
91.00	874.0
92.10	5733.0
93.10	9302.0
94.10	24464.0
95.10	194112.0
96.10	13373.0
97.10	252.0
103.00	120.0
104.00	1074.0
104.90	324.0
106.00	1073.0
106.90	165.0
110.00	245.0
111.00	184.0
111.90	137.0
112.90	162.0
114.90	220.0
115.90	863.0
117.00	1750.0
117.90	717.0
119.00	1168.0
124.00	168.0
128.00	748.0
129.00	388.0
130.00	712.0
131.00	285.0
135.00	514.0
137.00	336.0
141.00	2066.0
142.00	289.0
143.00	2404.0
143.90	113.0
145.00	572.0
146.00	358.0
148.00	328.0
149.00	154.0
150.00	196.0
152.10	103.0
155.00	478.0
157.00	323.0
159.00	194.0
161.00	238.0
170.40	115.0
171.10	376.0
172.10	1711.0
173.10	2134.0
174.10	136640.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

175.10	10877.0
176.10	133376.0
177.10	8499.0
178.00	245.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
36.00	2376.0
37.00	11908.0
38.10	10810.0
39.00	4288.0
40.00	357.0
43.00	109.0
44.00	1879.0
45.00	2036.0
46.10	275.0
47.00	2686.0
48.00	1290.0
49.10	10545.0
50.10	43352.0
51.10	13322.0
52.00	691.0
53.00	138.0
55.00	590.0
56.00	3482.0
57.10	6378.0
58.00	225.0
60.10	1956.0
61.10	11265.0
62.10	11956.0
63.10	9031.0
64.10	1147.0
65.10	1316.0
66.00	217.0
67.10	540.0
68.10	21856.0
69.10	23400.0
70.10	1892.0
72.10	1294.0
73.10	10523.0
74.10	39936.0
75.10	113208.0
76.10	9380.0
77.10	1354.0
78.00	920.0
79.00	8694.0
80.00	2856.0
81.00	9147.0
82.00	2339.0
83.00	175.0
85.90	216.0
87.10	8040.0
88.00	8927.0
91.00	951.0
92.10	6044.0
93.10	9758.0
94.10	26344.0
95.10	206080.0
96.10	13693.0
97.10	284.0
103.00	123.0
104.00	1209.0
104.90	347.0
106.00	1076.0
106.90	184.0
109.90	187.0
111.00	200.0
111.90	185.0
113.00	186.0
114.90	226.0
115.90	961.0
117.00	1709.0
117.90	773.0
119.00	1213.0
124.00	184.0
125.00	105.0
128.00	905.0
129.00	451.0
130.00	730.0
131.00	321.0
135.00	499.0
137.00	338.0
141.00	2312.0
142.00	280.0
143.00	2518.0
144.10	135.0
145.00	597.0
146.00	342.0
148.00	449.0
149.00	156.0
150.00	165.0
152.00	102.0
153.00	102.0
154.00	136.0
155.00	571.0
157.00	436.0
159.00	231.0
161.00	342.0
171.10	328.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

172.10	1771.0
174.10	149824.0
175.10	11639.0
176.10	145664.0
177.10	9029.0
178.00	279.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
36.00	2200.0
37.10	10986.0
38.10	9952.0
39.00	3989.0
40.00	383.0
43.00	135.0
44.00	1963.0
45.00	1948.0
47.00	2561.0
48.00	1272.0
49.00	10022.0
50.10	41128.0
51.10	12622.0
52.00	648.0
53.00	124.0
53.90	101.0
55.00	669.0
56.00	3175.0
57.00	6288.0
58.00	273.0
60.00	1898.0
61.10	10525.0
62.10	11404.0
63.10	8222.0
64.10	988.0
65.10	1058.0
66.00	193.0
67.10	464.0
68.10	20736.0
69.10	21680.0
70.10	1677.0
72.10	1237.0
73.10	10206.0
74.10	38216.0
75.10	107352.0
76.10	9126.0
77.10	1273.0
78.00	915.0
79.00	8079.0
80.00	2651.0
81.00	8671.0
82.00	2275.0
83.00	144.0
86.00	155.0
87.10	7824.0
88.10	8469.0
91.00	939.0
92.10	5893.0
93.10	9210.0
94.10	25216.0
95.10	198336.0
96.10	12862.0
97.10	334.0
103.00	111.0
104.00	1155.0
105.00	313.0
106.00	981.0
106.90	209.0
109.90	146.0
111.00	181.0
112.00	185.0
113.00	262.0
114.80	209.0
115.90	929.0
117.00	1527.0
117.90	755.0
119.00	1104.0
123.90	156.0
125.00	128.0
128.00	946.0
129.00	426.0
130.00	640.0
131.00	324.0
135.00	435.0
137.00	349.0
141.00	2353.0
142.00	272.0
143.00	2342.0
144.10	163.0
145.00	581.0
145.90	278.0
148.00	540.0
149.00	137.0
150.10	177.0
153.00	120.0
154.00	198.0
155.00	551.0
157.00	488.0
159.10	289.0
161.00	367.0
171.10	276.0
172.00	1653.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

174.10	146944.0
175.10	11262.0
176.10	143104.0
177.10	8559.0
178.00	313.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

Scan 2875 (10.584 min): VU040476.D
BFB13

m/z	Abundance
39.90	104.0
44.00	215.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13