

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU100323\  
 Data File : VU055651.D  
 Acq On : 03 Oct 2023 19:47  
 Operator : MD/SY  
 Sample : 04679-27  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VHBLK001

Quant Time: Oct 04 04:46:37 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR091923WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Oct 04 04:40:48 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.248  | 114   | 167380   | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 9.415  | 117   | 176563   | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.810 | 152   | 92646    | 5.000    | ug/L   | 0.00     |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.595  | 65    | 86491    | 5.113    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 102.200% |
| 7) Chloroethane-d5            | 1.911  | 69    | 68742    | 4.611    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 92.200%  |
| 11) 1,1-Dichloroethene-d2     | 2.563  | 65    | 34818    | 5.000    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 100.000% |
| 20) 2-Butanone-d5             | 4.627  | 46    | 147945   | 48.418   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 96.840%  |
| 24) Chloroform-d              | 5.058  | 84    | 142189   | 4.647    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 93.000%  |
| 26) 1,2-Dichloroethane-d4     | 5.698  | 65    | 71516    | 4.859    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 97.200%  |
| 32) Benzene-d6                | 5.724  | 84    | 287501   | 4.655    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 93.200%  |
| 36) 1,2-Dichloropropane-d6    | 6.688  | 67    | 87695    | 4.753    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 95.000%  |
| 41) Toluene-d8                | 7.897  | 98    | 246446   | 4.378    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 87.600%  |
| 43) trans-1,3-Dichloroprop... | 8.180  | 79    | 30912    | 4.774    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 95.400%  |
| 46) 2-Hexanone-d5             | 8.631  | 63    | 84528    | 42.915   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 85.820%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.756 | 84    | 64091    | 4.635    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 92.600%  |
| 66) 1,2-Dichlorobenzene-d4    | 12.190 | 152   | 85769    | 4.587    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 91.800%  |
| Target Compounds              |        |       |          |          |        |          |
|                               |        |       |          |          | Qvalue |          |
| 16) Methylene chloride        | 3.046  | 84    | 5606     | 0.400    | ug/L   | 91       |
| 70) 1,2,4-trichlorobenzene    | 13.843 | 180   | 19946    | 1.486    | ug/L   | 97       |
| -----                         |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU100323\  
Data File : VU055651.D  
Acq On : 03 Oct 2023 19:47  
Operator : MD/SY  
Sample : 04679-27  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VHBLK001

Quant Time: Oct 04 04:46:37 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR091923WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Wed Oct 04 04:40:48 2023  
Response via : Initial Calibration




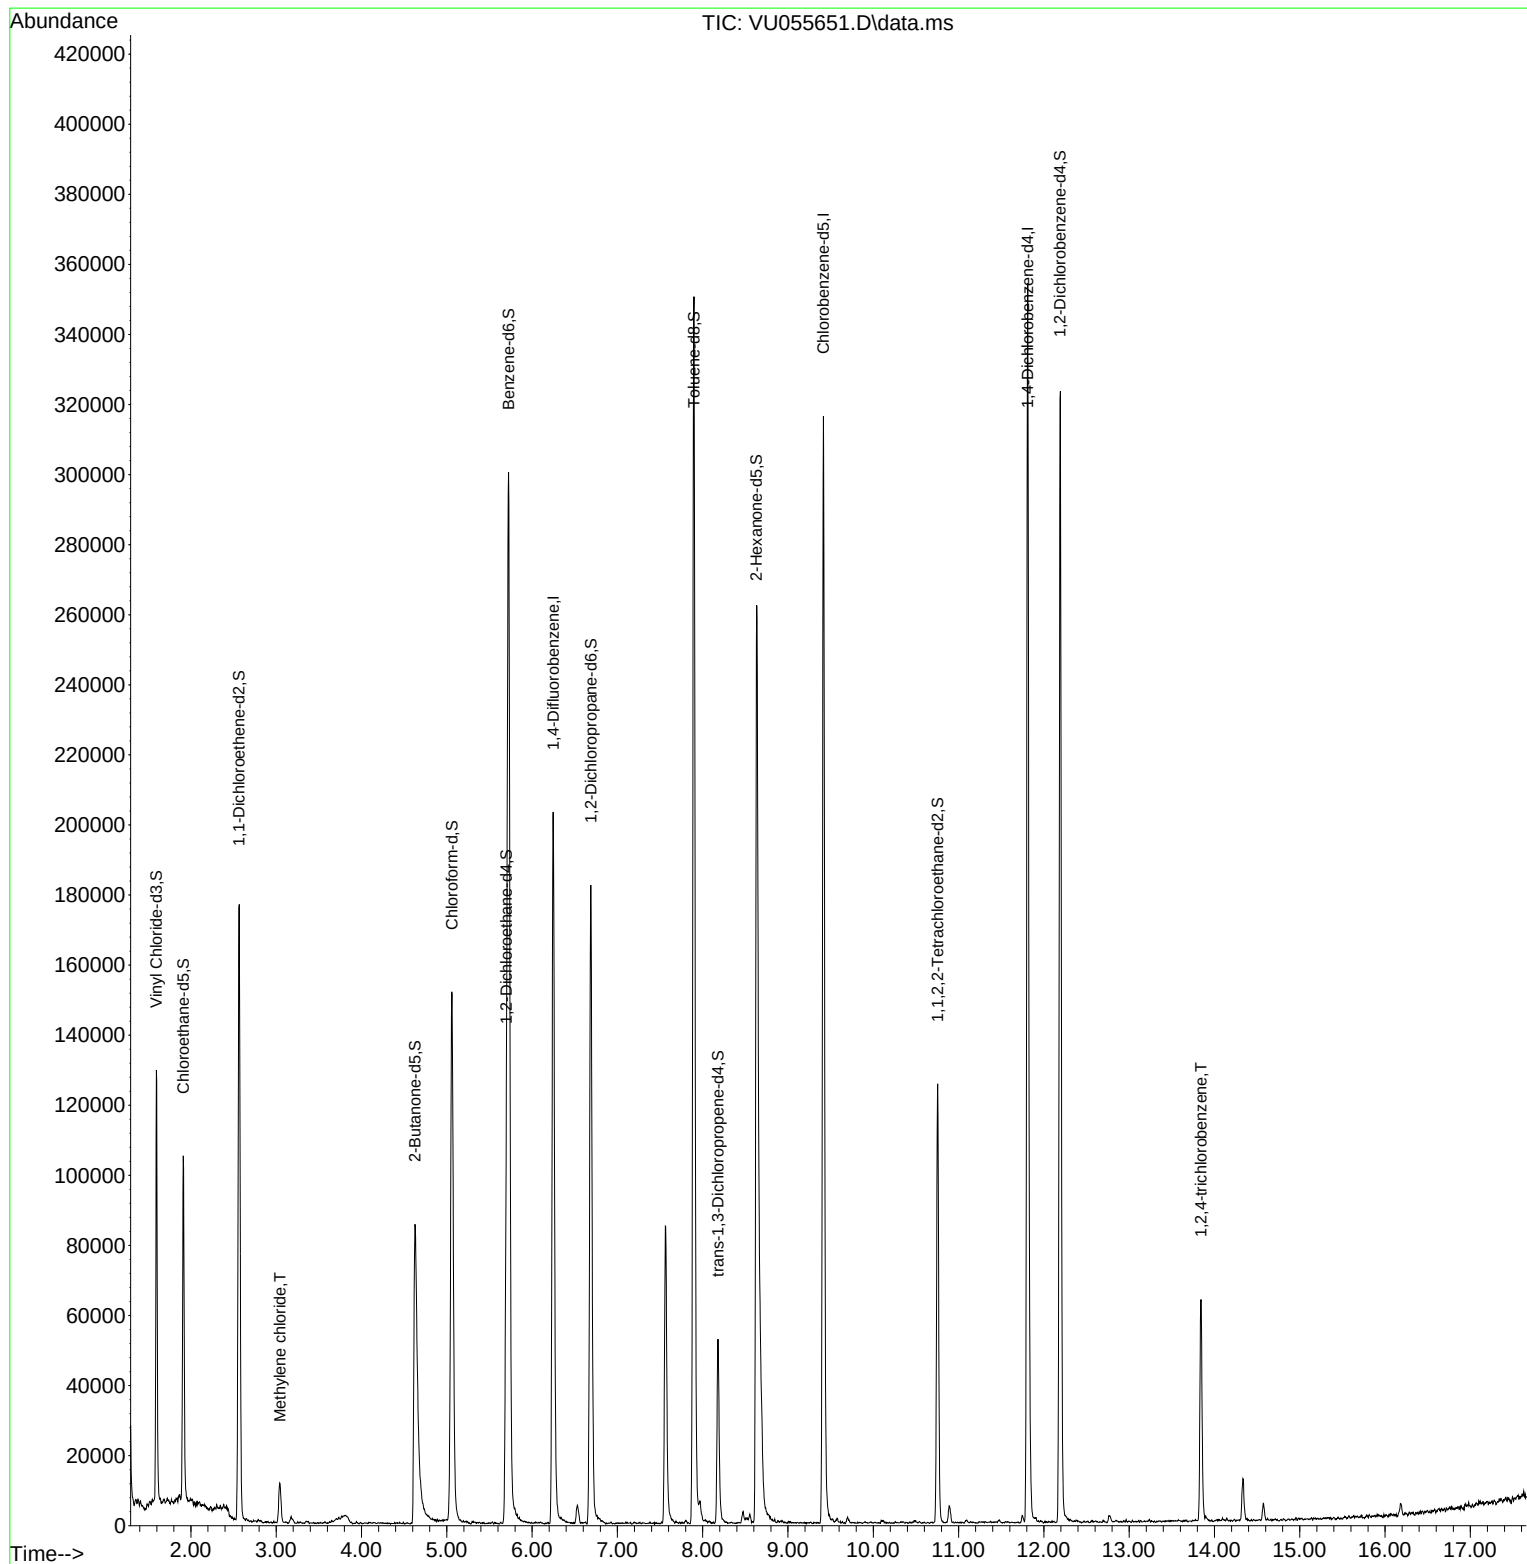


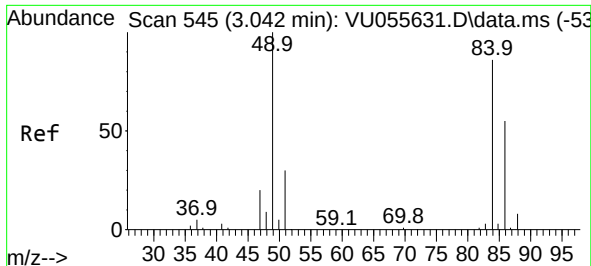

#16  
Methylene chloride  
Concen: 0.400 ug/L  
RT: 3.046 min Scan# 54  
Delta R.T. 0.003 min  
Lab File: VU055651.D  
Acq: 03 Oct 2023 19:47

Instrument :  
MSVOA\_U  
ClientSampleId :  
VHBLK001

Tgt Ion: 84 Resp: 5606  
Ion Ratio Lower Upper  
84 100  
86 62.5 44.9 83.3  
49 126.0 78.8 146.3

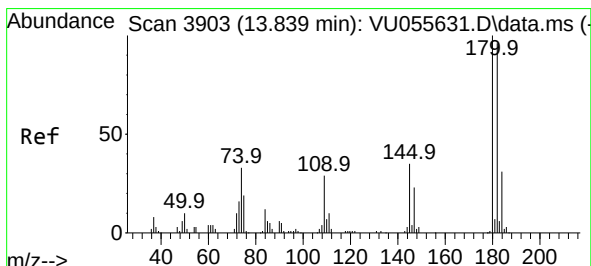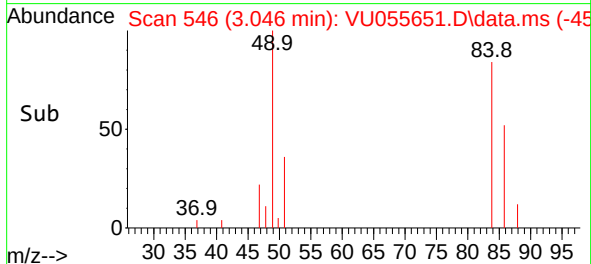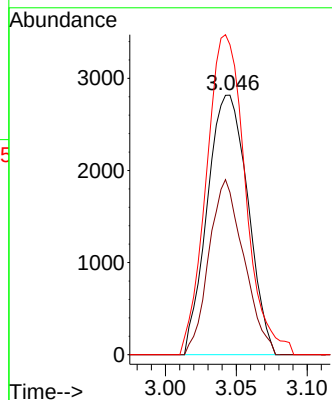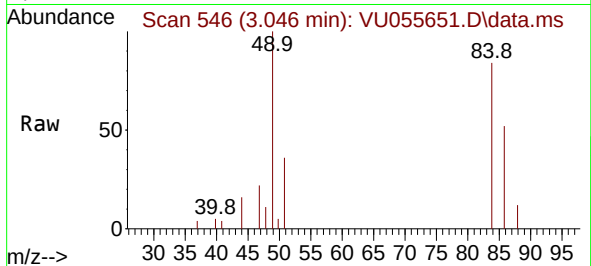

#70  
1,2,4-trichlorobenzene  
Concen: 1.486 ug/L  
RT: 13.843 min Scan# 3904  
Delta R.T. 0.003 min  
Lab File: VU055651.D  
Acq: 03 Oct 2023 19:47

Tgt Ion:180 Resp: 19946  
Ion Ratio Lower Upper  
180 100  
182 98.8 76.4 114.6  
145 32.9 25.4 38.0

