

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
 Data File : VU055632.D
 Acq On : 03 Oct 2023 11:33
 Operator : MD/SY
 Sample : VU1003WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	106	rBV	127499	146749	18.80%	2.394%
2	1.914	185	194	207	rVB	108071	141295	18.10%	2.305%
3	2.566	384	397	417	rBV	184111	303473	38.87%	4.951%
4	3.039	535	544	562	rBV2	9946	18726	2.40%	0.305%
5	4.631	1023	1039	1078	rBV	72888	230697	29.55%	3.764%
6	5.062	1154	1173	1195	rBV	151923	338552	43.36%	5.523%
7	5.724	1359	1379	1409	rBV2	300953	780783	100.00%	12.738%
8	6.248	1529	1542	1565	rBV	213697	424868	54.42%	6.931%
9	6.534	1619	1631	1640	rBV8	4925	10145	1.30%	0.166%
10	6.688	1665	1679	1701	rBV	179810	363332	46.53%	5.927%
11	7.566	1938	1952	1972	rBV2	84888	160035	20.50%	2.611%
12	7.897	2041	2055	2070	rBV	361661	647489	82.93%	10.563%
13	8.180	2132	2143	2160	rBV	49832	90018	11.53%	1.469%
14	8.637	2272	2285	2321	rBV4	221541	563196	72.13%	9.188%
15	9.418	2515	2528	2547	rBV	326838	566787	72.59%	9.247%
16	10.753	2930	2943	2961	rBV	114201	189585	24.28%	3.093%
17	11.810	3260	3272	3294	rBV	350304	597856	76.57%	9.753%
18	12.193	3377	3391	3412	rBV	304095	522808	66.96%	8.529%
19	13.849	3896	3906	3919	rBV3	8555	14695	1.88%	0.240%
20	14.100	3975	3984	3994	rBV3	4402	7971	1.02%	0.130%
21	14.331	4049	4056	4066	rBV6	6500	10631	1.36%	0.173%




Sum of corrected areas: 6129691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
Data File : VU055632.D
Acq On : 03 Oct 2023 11:33
Operator : MD/SY
Sample : VU1003WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

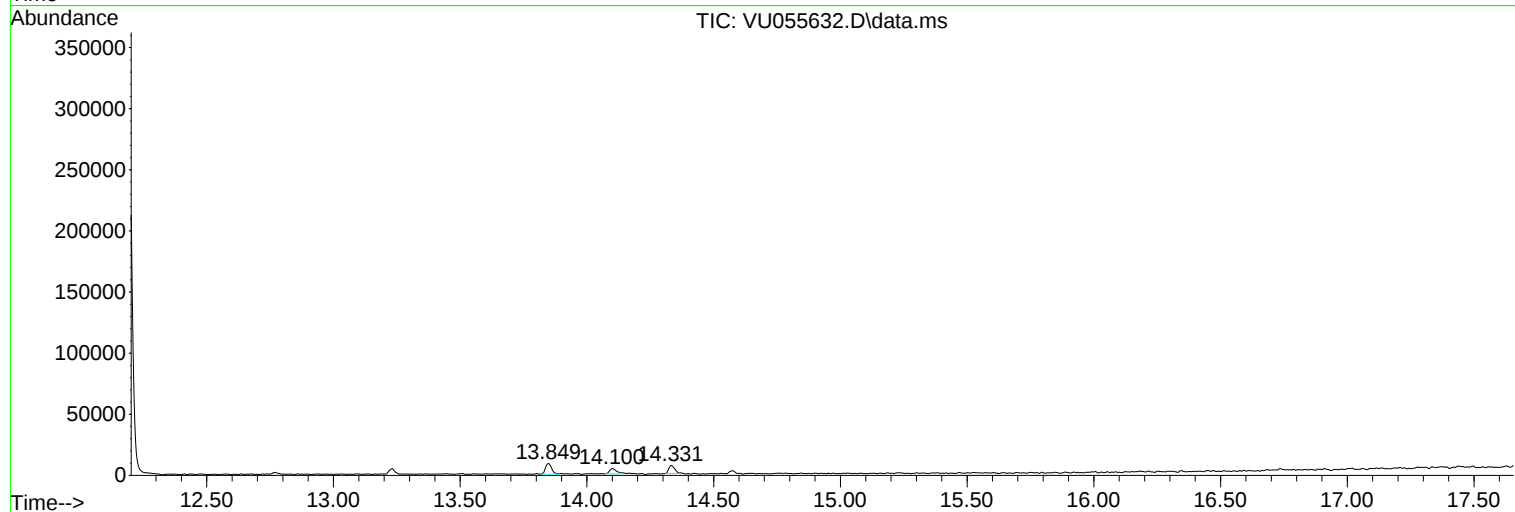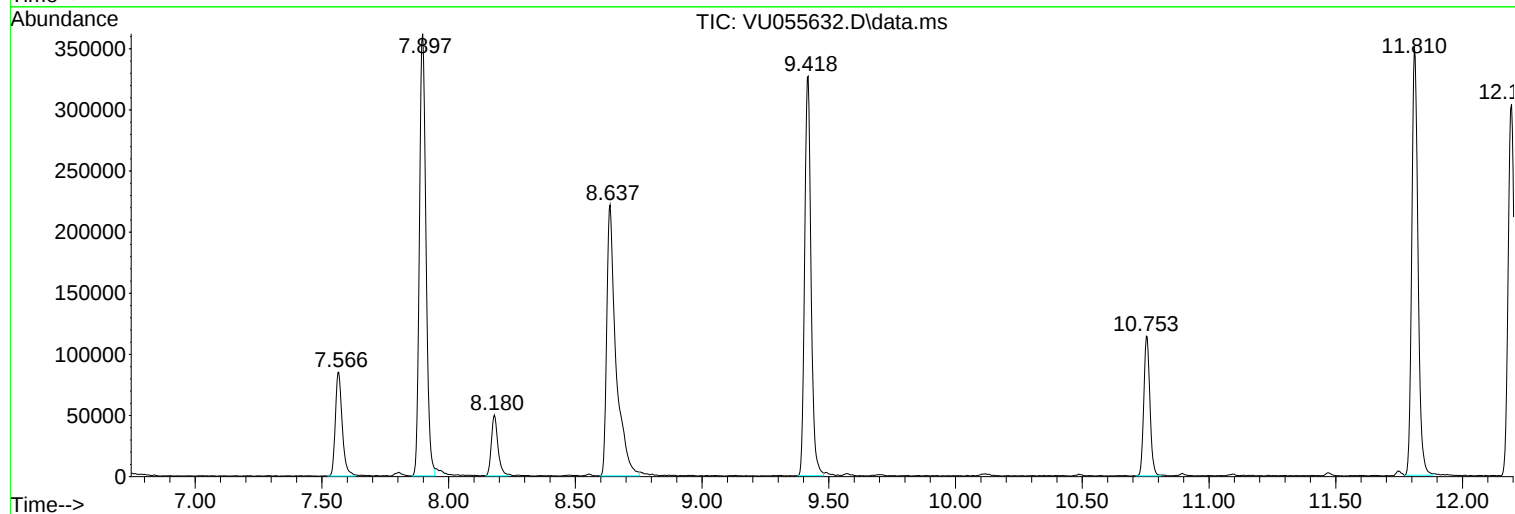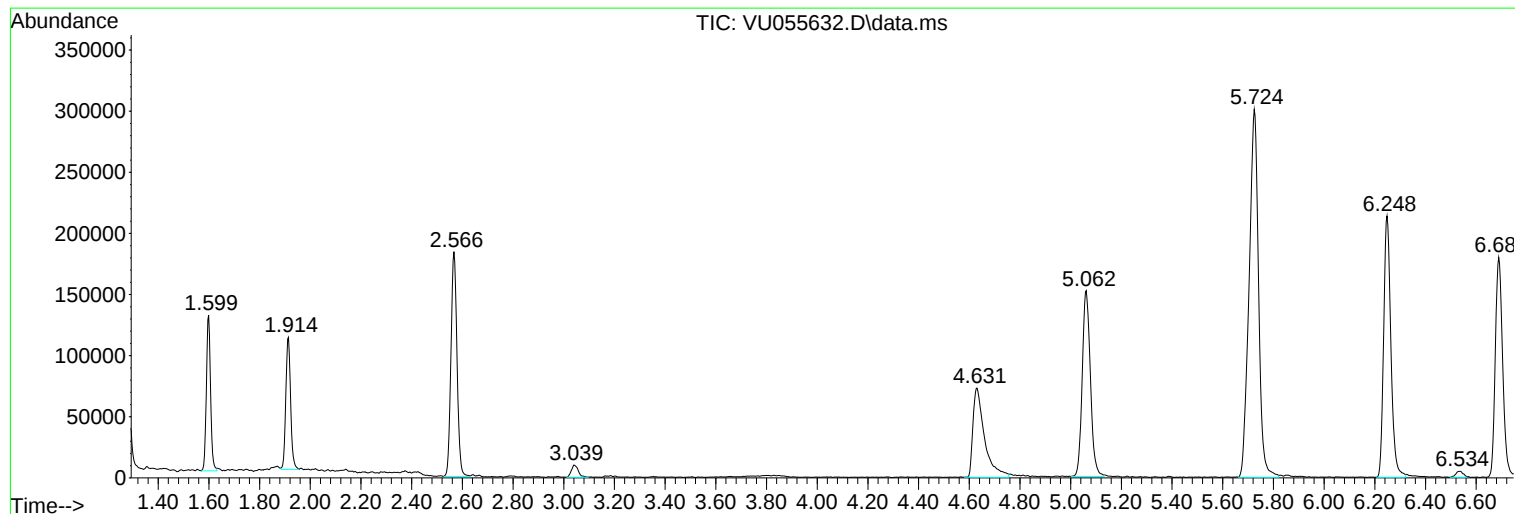

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
Data File : VU055632.D
Acq On : 03 Oct 2023 11:33
Operator : MD/SY
Sample : VU1003WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
Data File : VU055632.D
Acq On : 03 Oct 2023 11:33
Operator : MD/SY
Sample : VU1003WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc