

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
 Data File : VU055638.D
 Acq On : 03 Oct 2023 14:05
 Operator : MD/SY
 Sample : 04679-26DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7D(20230928)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	110	rBV	132204	149156	14.80%	2.189%
2	1.914	185	194	210	rVB	107879	136533	13.54%	2.004%
3	2.566	384	397	416	rBV	183821	301907	29.95%	4.431%
4	3.042	533	545	563	rVB	27853	52815	5.24%	0.775%
5	3.869	788	802	814	rVB4	4742	13423	1.33%	0.197%
6	4.631	1024	1039	1081	rBV3	77172	284375	28.21%	4.173%
7	5.062	1154	1173	1200	rBV	150690	345009	34.23%	5.063%
8	5.724	1359	1379	1410	rBV2	304903	792171	78.58%	11.625%
9	6.248	1528	1542	1562	rBV	217113	421477	41.81%	6.185%
10	6.688	1664	1679	1701	rBV	182430	364124	36.12%	5.344%
11	7.563	1939	1951	1973	rBV2	87933	162271	16.10%	2.381%
12	7.897	2042	2055	2072	rBV	370306	655786	65.05%	9.624%
13	8.180	2132	2143	2160	rBV2	49400	89501	8.88%	1.313%
14	8.634	2273	2284	2320	rBV4	229098	573433	56.89%	8.415%
15	9.415	2514	2527	2551	rBV	326847	614518	60.96%	9.018%
16	10.753	2928	2943	2962	rBV2	118003	194836	19.33%	2.859%
17	11.746	3242	3252	3261	rBV2	52740	84907	8.42%	1.246%
18	11.810	3261	3272	3296	rVB2	392591	1008049	100.00%	14.793%
19	12.190	3376	3390	3411	rBV	328018	557806	55.34%	8.186%
20	13.849	3896	3906	3918	rBV3	7093	12177	1.21%	0.179%




Sum of corrected areas: 6814274

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
Data File : VU055638.D
Acq On : 03 Oct 2023 14:05
Operator : MD/SY
Sample : 04679-26DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7D(20230928)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

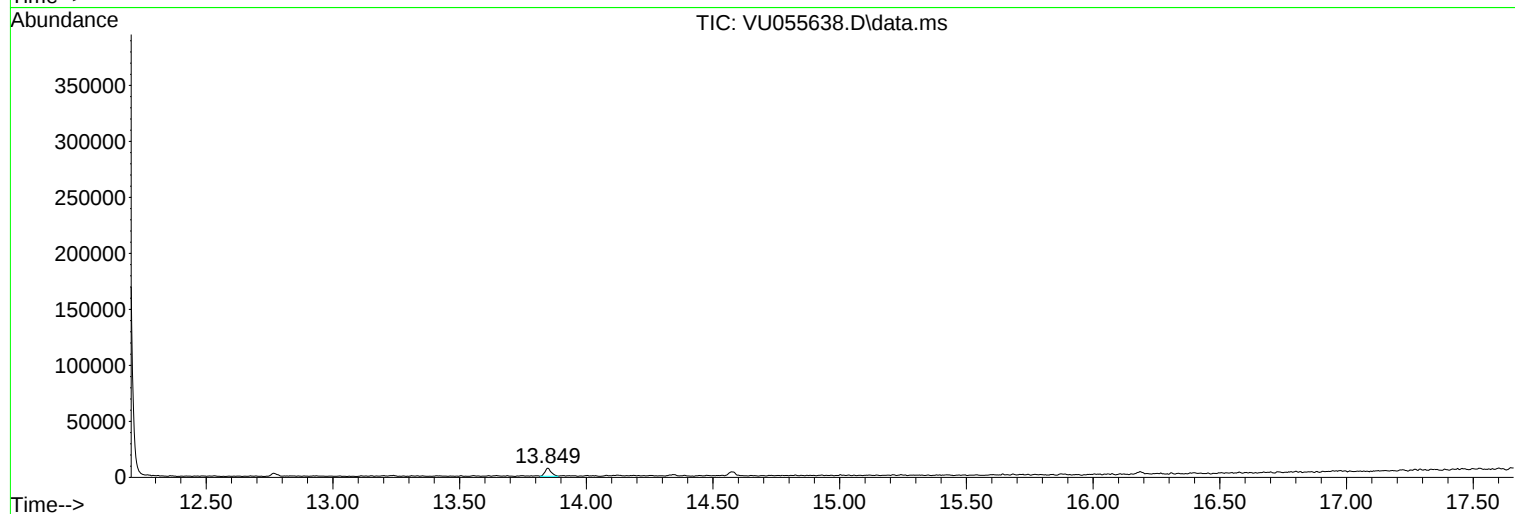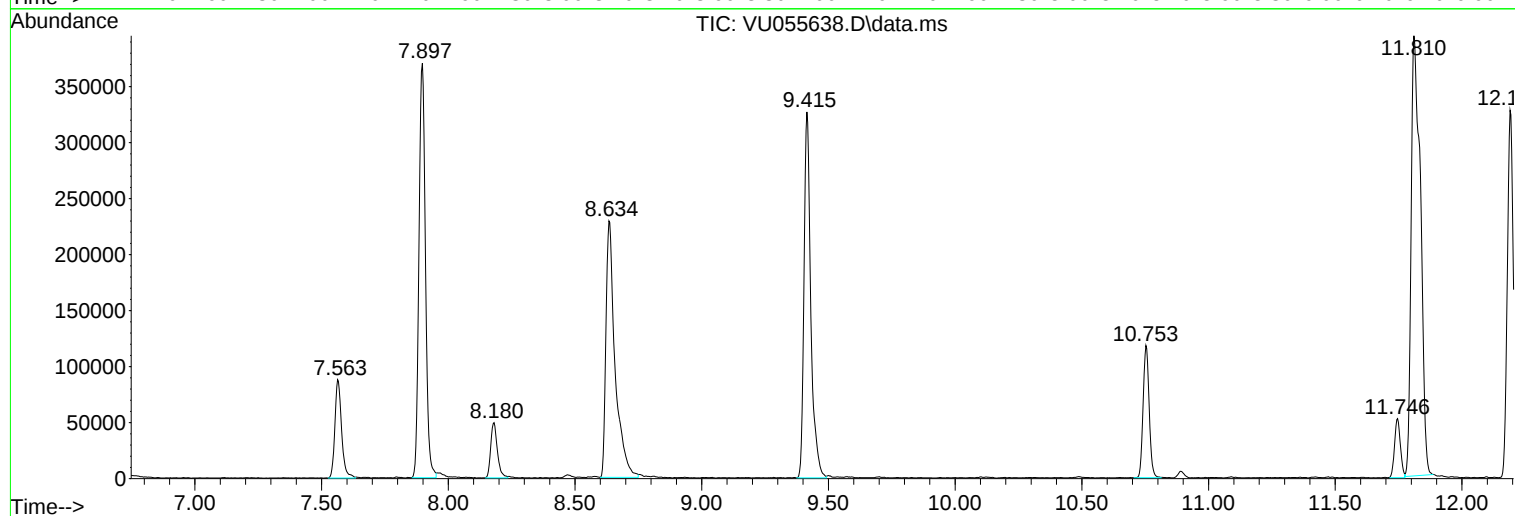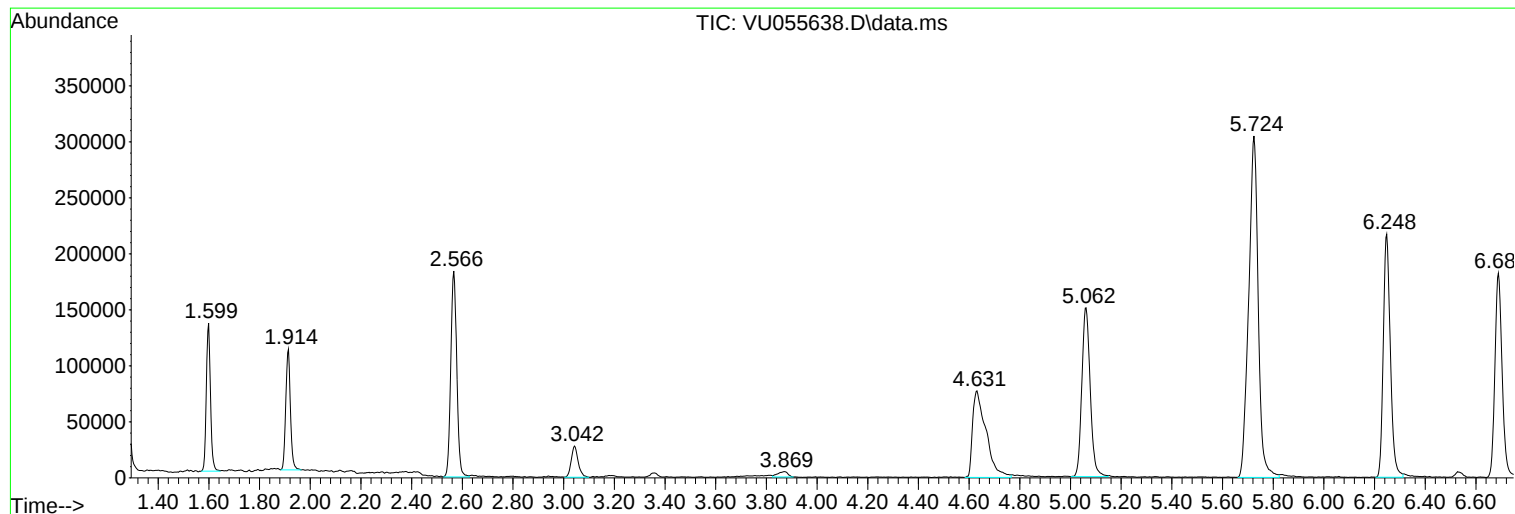

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
Data File : VU055638.D
Acq On : 03 Oct 2023 14:05
Operator : MD/SY
Sample : 04679-26DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7D(20230928)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
Data File : VU055638.D
Acq On : 03 Oct 2023 14:05
Operator : MD/SY
Sample : 04679-26DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7D(20230928)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------