

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
 Data File : VU055648.D
 Acq On : 03 Oct 2023 18:34
 Operator : MD/SY
 Sample : 04679-15DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7S(20230927)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	110	rBV	125683	145384	10.03%	1.983%
2	1.911	185	193	205	rBV	92338	120289	8.30%	1.641%
3	2.566	384	397	419	rBV	176745	291311	20.10%	3.974%
4	3.042	530	545	560	rBV2	67938	129838	8.96%	1.771%
5	3.354	630	642	657	rVB3	7996	15660	1.08%	0.214%
6	4.660	1029	1048	1071	rBV2	92298	352283	24.31%	4.806%
7	5.062	1155	1173	1193	rBV	142645	329241	22.72%	4.492%
8	5.724	1357	1379	1414	rBV3	290250	760185	52.46%	10.371%
9	6.248	1527	1542	1565	rBV	200970	391288	27.00%	5.338%
10	6.688	1664	1679	1698	rBV	171611	347573	23.98%	4.742%
11	7.566	1936	1952	1980	rBV	81808	155516	10.73%	2.122%
12	7.897	2039	2055	2071	rBV	351400	617686	42.62%	8.427%
13	8.180	2131	2143	2163	rBV	48651	88097	6.08%	1.202%
14	8.637	2273	2285	2320	rBV3	238915	585629	40.41%	7.990%
15	9.415	2513	2527	2553	rBV2	303699	611675	42.21%	8.345%
16	10.753	2930	2943	2960	rBV	121688	197803	13.65%	2.699%
17	10.894	2973	2987	2996	rBV3	10260	17806	1.23%	0.243%
18	11.746	3238	3252	3262	rBV	106039	170999	11.80%	2.333%
19	11.833	3262	3279	3301	rVB2	578627	1449135	100.00%	19.771%
20	12.193	3378	3391	3412	rBV	320163	552285	38.11%	7.535%




Sum of corrected areas: 7329683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
Data File : VU055648.D
Acq On : 03 Oct 2023 18:34
Operator : MD/SY
Sample : 04679-15DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7S(20230927)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

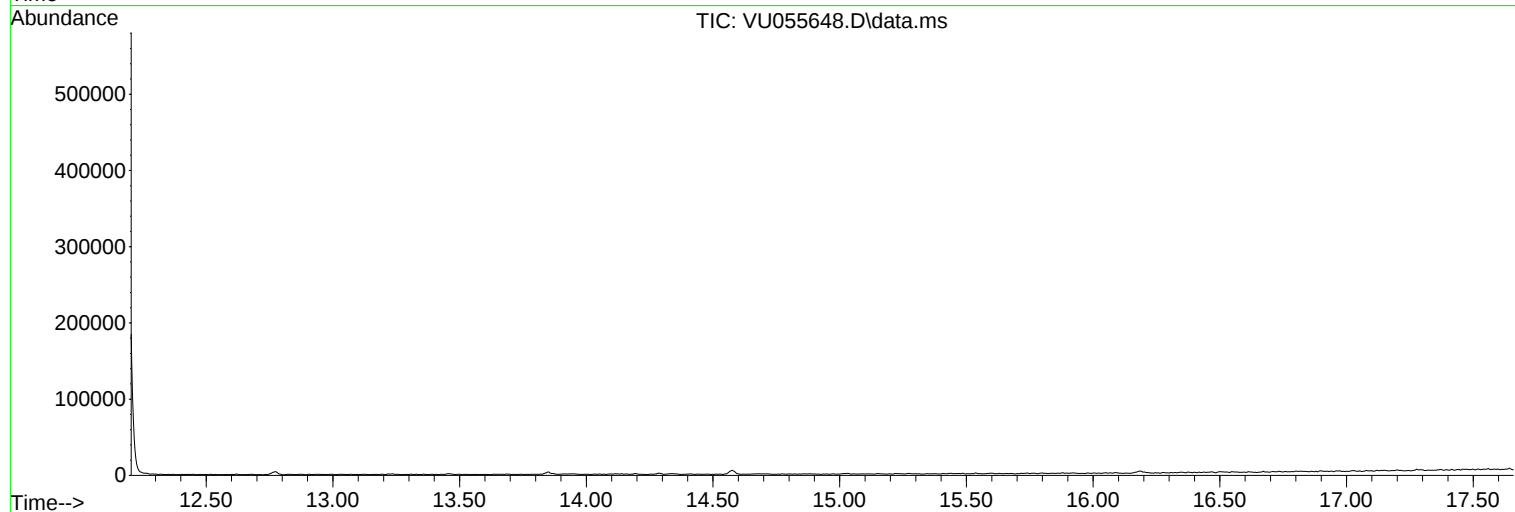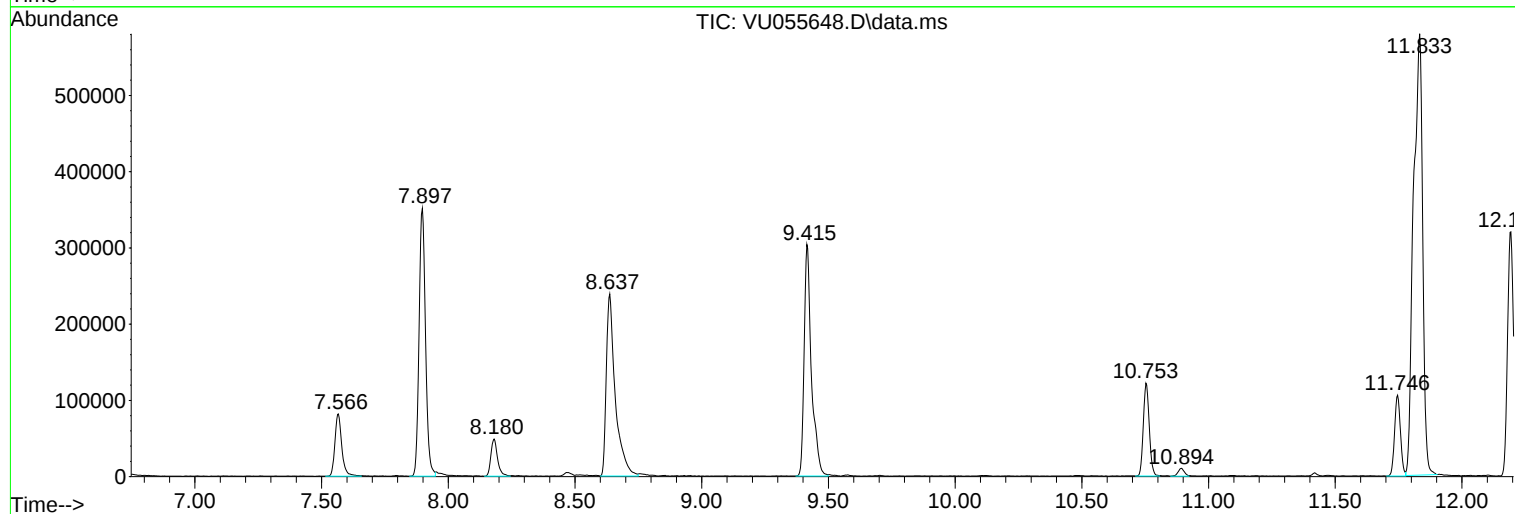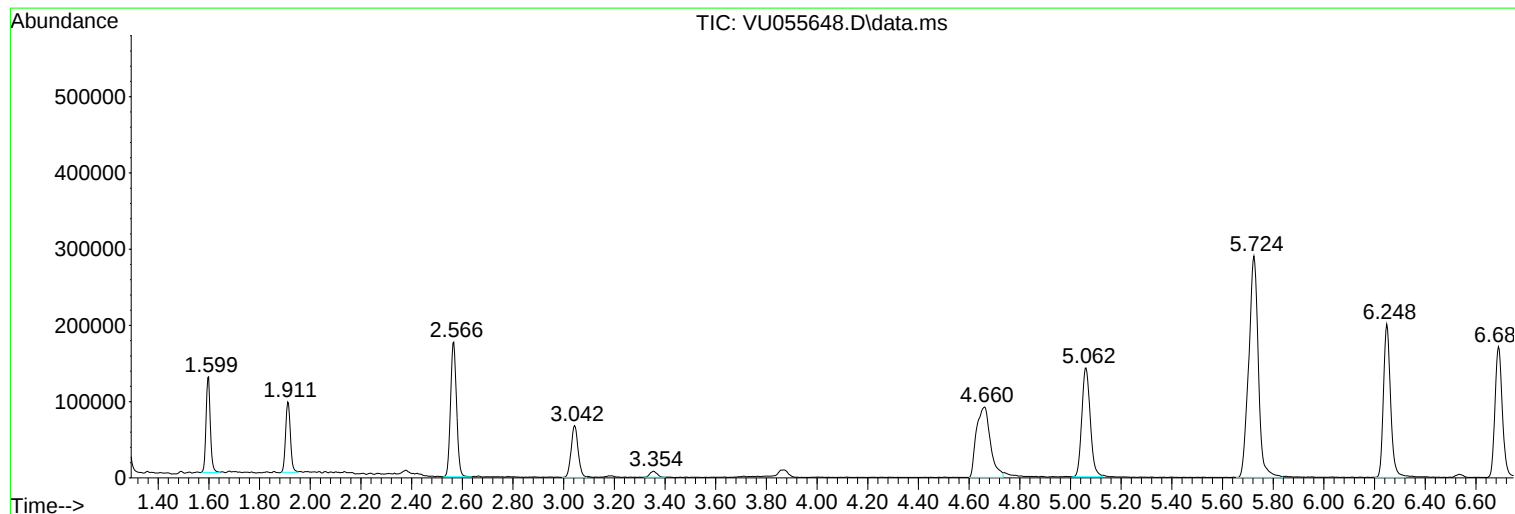

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
Data File : VU055648.D
Acq On : 03 Oct 2023 18:34
Operator : MD/SY
Sample : 04679-15DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7S(20230927)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
Data File : VU055648.D
Acq On : 03 Oct 2023 18:34
Operator : MD/SY
Sample : 04679-15DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7S(20230927)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------