


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100323\
Data File : VU055629.D
Acq On : 03 Oct 2023 08:46
Operator : MD/SY
Sample : BFB056
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB056

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Oct 04 23:00:34 2023

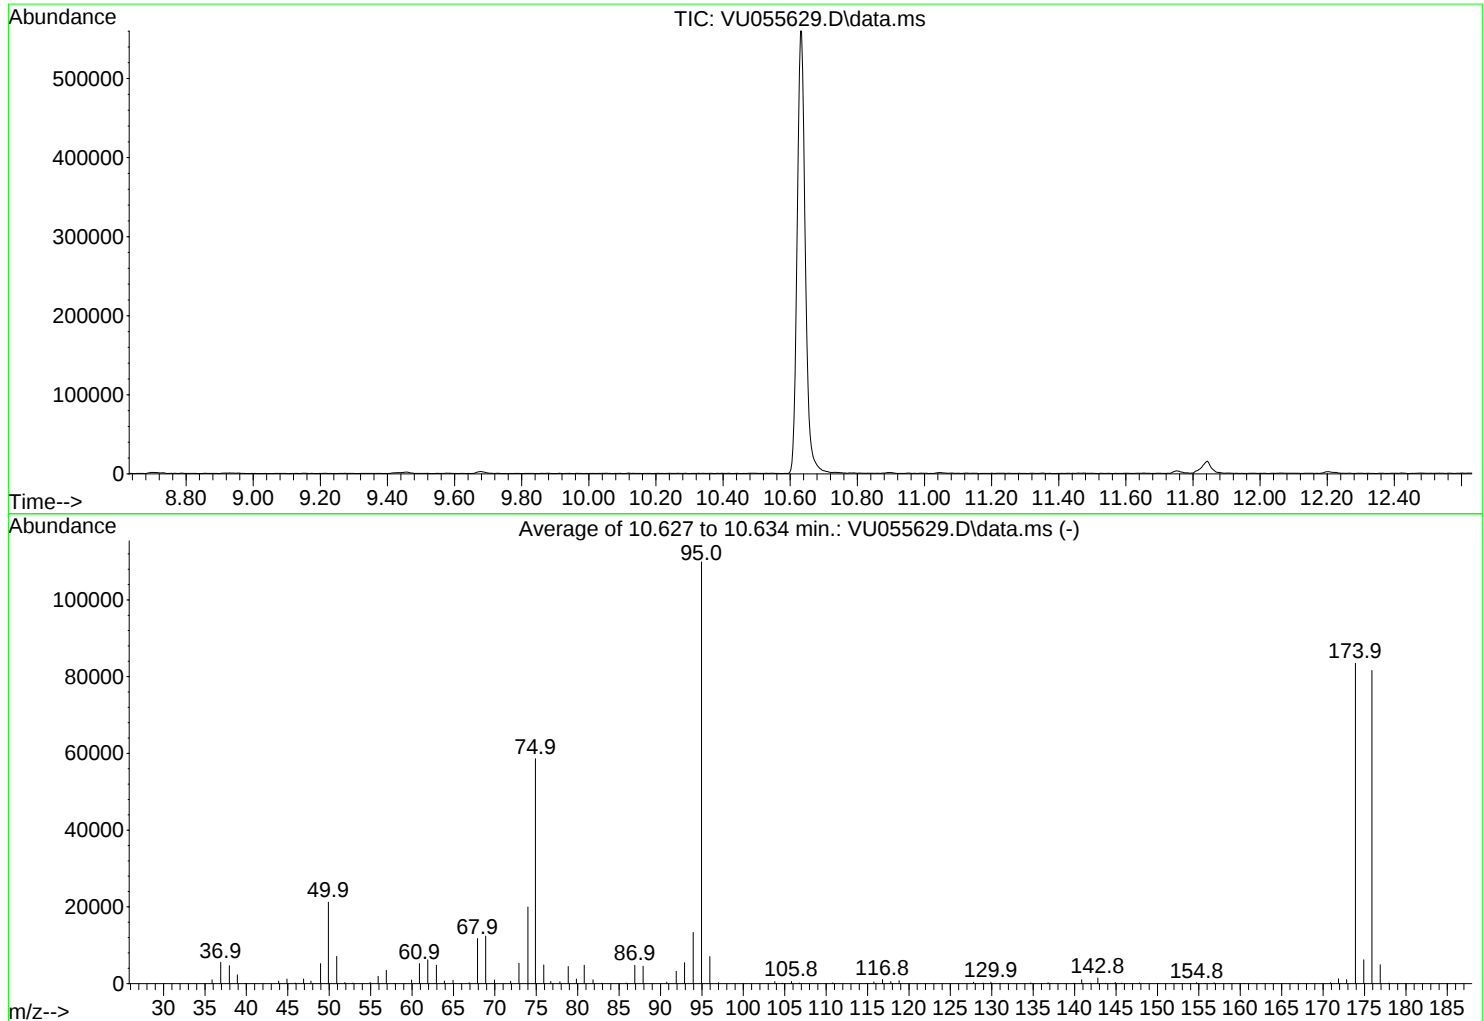

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	21229	PASS
75	95	30	80	53.3	58619	PASS
95	95	100	100	100.0	109912	PASS
96	95	5	9	6.4	7069	PASS
173	174	0.00	2	1.3	1049	PASS
174	95	50	120	75.9	83472	PASS
175	174	5	9	7.5	6234	PASS
176	174	95	101	97.7	81581	PASS
177	176	5	9	6.0	4908	PASS

m/z	Abundance
39.80	159.0
43.90	546.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
35.90	1109.0
36.90	5345.0
38.00	4589.0
38.90	2260.0
39.90	196.0
43.90	1307.0
44.90	1252.0
45.90	209.0
46.90	1166.0
47.80	625.0
49.00	5170.0
49.90	20248.0
50.90	6619.0
51.90	255.0
52.90	142.0
55.00	335.0
55.90	1999.0
56.90	3411.0
57.80	121.0
59.90	917.0
60.90	4711.0
61.90	5938.0
63.00	4433.0
64.00	712.0
64.90	789.0
66.90	268.0
67.90	11237.0
68.90	11908.0
69.90	859.0
71.90	513.0
72.90	5074.0
74.00	19520.0
74.90	54608.0
75.90	4726.0
76.80	559.0
77.90	499.0
78.80	4091.0
79.80	1137.0
80.80	4645.0
81.90	1004.0
82.90	120.0
85.80	114.0
86.90	4637.0
87.90	4137.0
90.80	516.0
91.90	3120.0
92.90	5123.0
94.00	13120.0
95.00	104080.0
96.00	6720.0
97.00	222.0
103.80	508.0
105.80	490.0
106.70	126.0
110.80	151.0
114.80	123.0
115.80	436.0
116.80	929.0
117.80	530.0
118.80	612.0
127.80	305.0
129.00	127.0
129.90	346.0
134.60	210.0
136.80	197.0
139.90	103.0
140.90	893.0
141.90	113.0
142.80	1295.0
143.70	136.0
144.90	276.0
145.70	144.0
147.80	229.0
154.80	237.0
156.90	161.0
160.50	107.0
170.90	279.0
171.80	1116.0
172.90	984.0
173.90	76816.0
174.90	5984.0
175.90	73760.0
176.90	4554.0
178.00	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
35.80	1055.0
36.90	5711.0
38.00	4869.0
38.90	2342.0
39.90	192.0
43.90	1212.0
44.90	1285.0
45.90	198.0
46.90	1258.0
47.80	712.0
48.90	5411.0
49.90	21800.0
50.90	7401.0
51.90	337.0
52.90	142.0
55.00	303.0
55.90	1941.0
56.90	3565.0
57.90	118.0
60.00	969.0
60.90	5350.0
61.90	6426.0
63.00	4955.0
63.90	640.0
65.00	924.0
65.90	120.0
66.90	270.0
67.90	12125.0
68.90	12847.0
70.00	1019.0
71.90	641.0
72.90	5524.0
74.00	20632.0
74.90	60528.0
75.90	4998.0
76.70	596.0
77.80	543.0
78.90	4579.0
79.80	1211.0
80.80	4978.0
81.90	1037.0
82.90	134.0
85.90	142.0
86.90	4951.0
87.90	4759.0
90.80	412.0
91.90	3346.0
92.90	5635.0
93.90	13658.0
95.00	113248.0
95.90	7321.0
97.00	274.0
103.80	581.0
104.70	161.0
105.80	609.0
106.70	164.0
110.80	233.0
115.70	475.0
116.80	1084.0
117.80	568.0
118.80	810.0
127.80	400.0
129.00	160.0
129.90	393.0
131.00	126.0
134.70	217.0
136.80	236.0
139.90	134.0
140.90	1048.0
141.90	164.0
142.80	1530.0
143.80	135.0
144.90	360.0
145.70	170.0
146.80	121.0
147.80	235.0
154.80	289.0
155.80	100.0
156.80	251.0
158.70	135.0
170.90	303.0
171.90	1268.0
172.80	1073.0
173.90	85792.0
174.90	6493.0
175.90	84384.0
176.90	5086.0
178.00	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
35.90	903.0
36.90	5541.0
37.90	4698.0
38.90	2229.0
39.90	229.0
43.90	1063.0
44.90	1142.0
45.90	125.0
46.90	1189.0
47.80	721.0
48.90	5090.0
49.90	21640.0
50.90	7244.0
51.90	316.0
52.80	162.0
54.80	347.0
55.90	1804.0
56.90	3371.0
60.00	1033.0
60.90	5624.0
61.90	6246.0
62.90	5041.0
63.80	649.0
65.00	939.0
65.90	121.0
66.90	273.0
67.90	11947.0
68.90	12351.0
70.00	1054.0
71.90	696.0
72.90	5404.0
74.00	19776.0
74.90	60720.0
75.90	4975.0
76.80	639.0
77.80	508.0
78.90	4750.0
79.90	1336.0
80.80	4743.0
81.80	1008.0
82.90	145.0
85.90	222.0
86.90	4756.0
87.90	4739.0
90.70	331.0
91.90	3200.0
92.90	5618.0
93.90	13250.0
94.90	112408.0
95.90	7167.0
97.00	266.0
103.80	608.0
104.70	238.0
105.80	688.0
106.80	168.0
110.80	243.0
115.70	515.0
116.80	1082.0
117.80	566.0
118.80	939.0
127.80	445.0
128.90	164.0
129.90	447.0
131.00	144.0
134.80	189.0
136.80	265.0
139.90	156.0
140.80	1109.0
141.90	174.0
142.80	1607.0
143.80	135.0
144.90	426.0
145.70	147.0
147.90	206.0
154.70	309.0
155.80	124.0
156.80	283.0
158.60	133.0
170.90	244.0
171.90	1363.0
172.80	1090.0
173.90	87808.0
174.90	6225.0
175.90	86600.0
176.90	5085.0
177.90	182.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056