

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100418\
 Data File : VU027426.D
 Acq On : 04 Oct 2018 22:20
 Operator : MD/SY
 Sample : J5232-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-8

Quant Time: Oct 08 11:04:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 02 02:04:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	106115	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	185604	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	178782	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	95300	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.31	65	103182	58.23	ug/l	0.00
Spiked Amount			Recovery	=	116.46%	
35) Dibromofluoromethane	4.89	113	74137	58.28	ug/l	0.00
Spiked Amount			Recovery	=	116.56%	
50) Toluene-d8	7.57	98	285970	60.07	ug/l	0.00
Spiked Amount			Recovery	=	120.14%	
62) 4-Bromofluorobenzene	10.31	95	102998	58.22	ug/l	0.00
Spiked Amount			Recovery	=	116.44%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100418\
Data File : VU027426.D
Acq On : 04 Oct 2018 22:20
Operator : MD/SY
Sample : J5232-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-8

Quant Time: Oct 08 11:04:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 02 02:04:34 2018
Response via : Initial Calibration

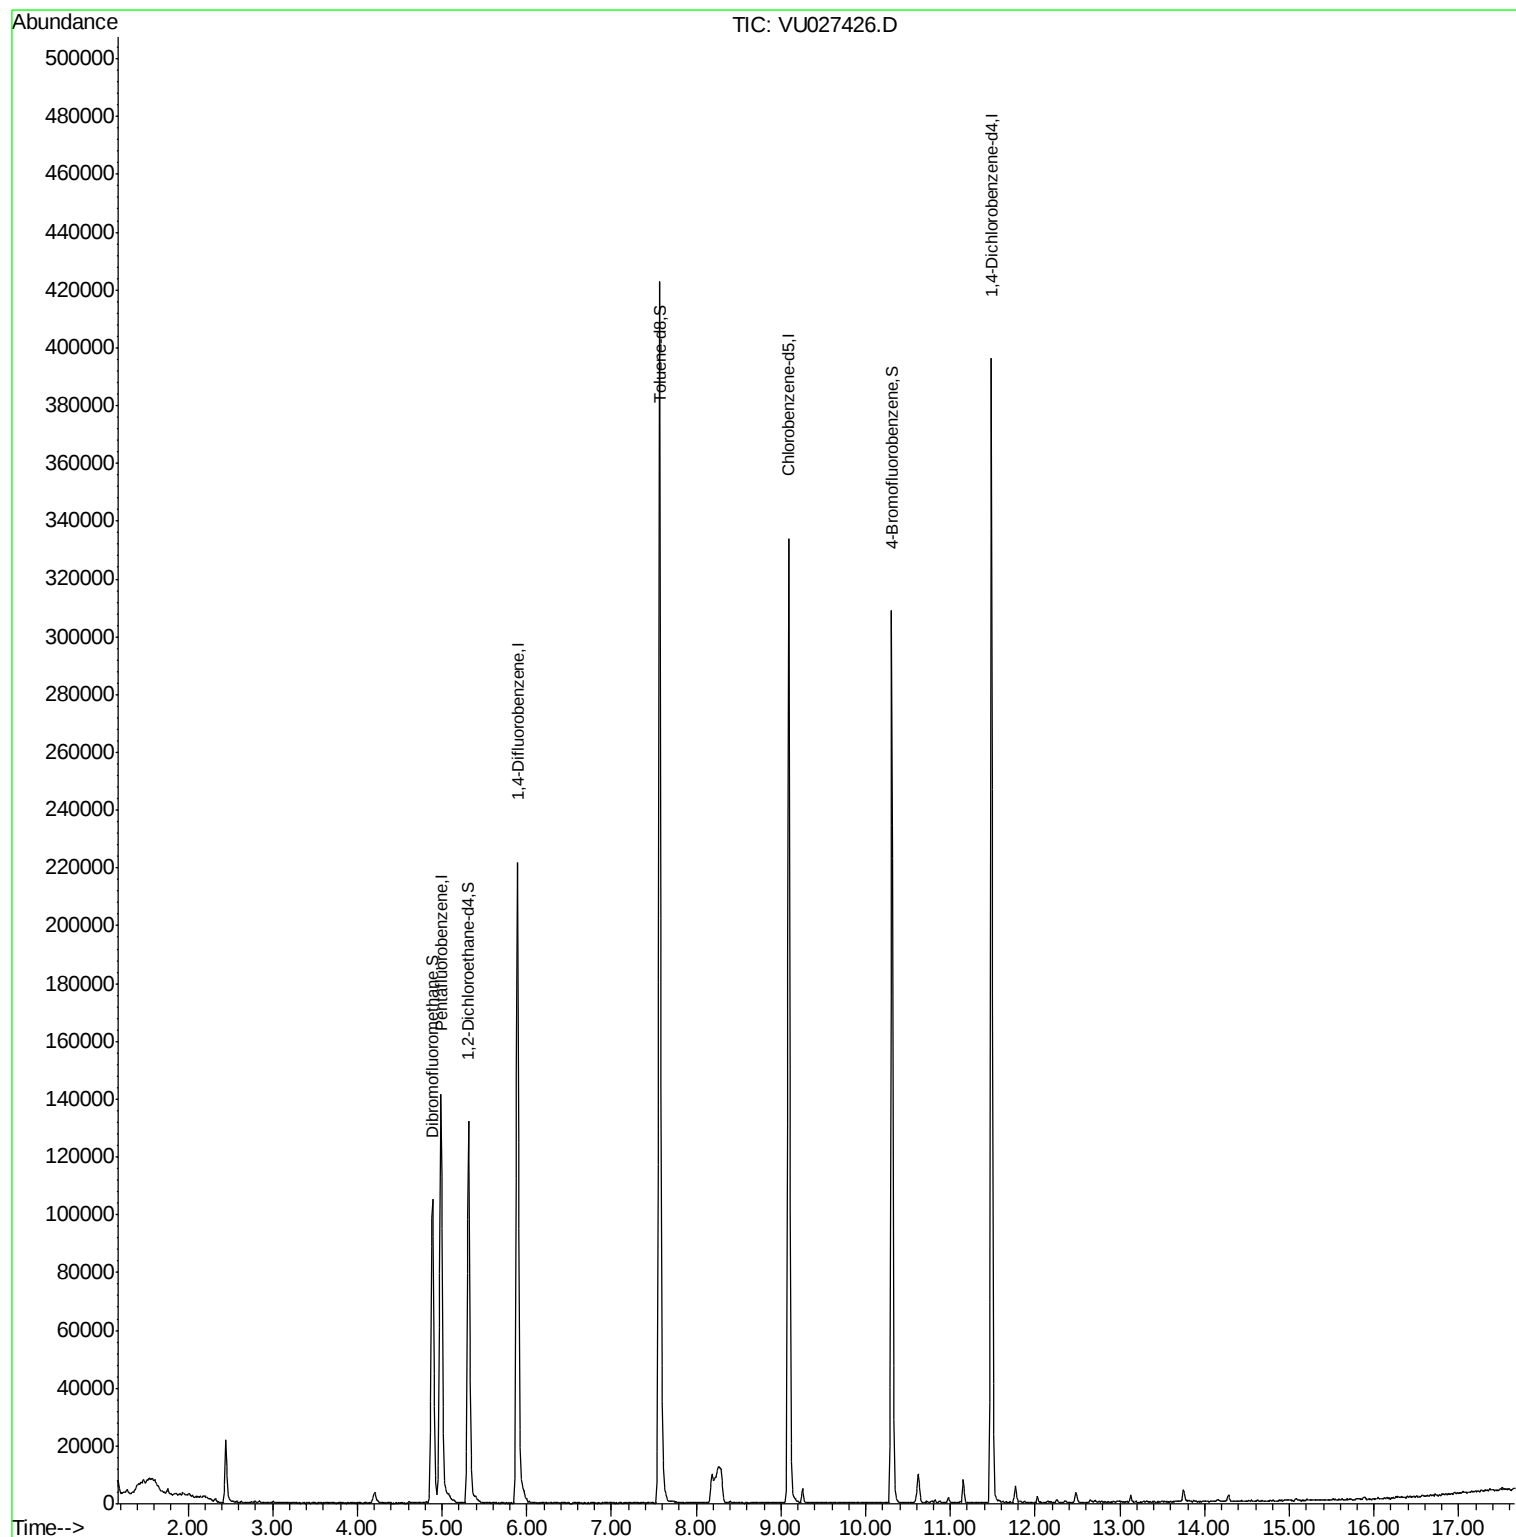

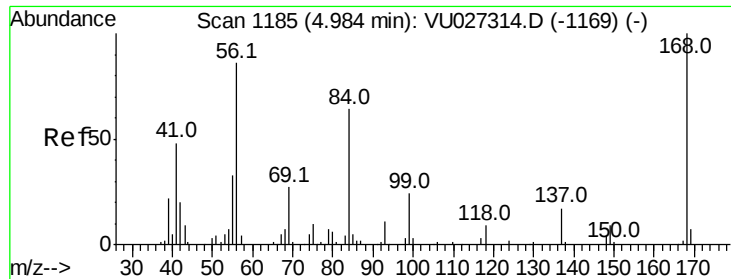

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.99 min Scan# 1186

Delta R.T. 0.00 min

Lab File: VU027426.D

Acq: 04 Oct 2018 22:20

Instrument :

MSVOA_U

ClientSampleId :


MW-8

Tot Ion:168 Resp: 106115

Ion Ratio Lower Upper

168 100

99 62.0 50.8 76.2



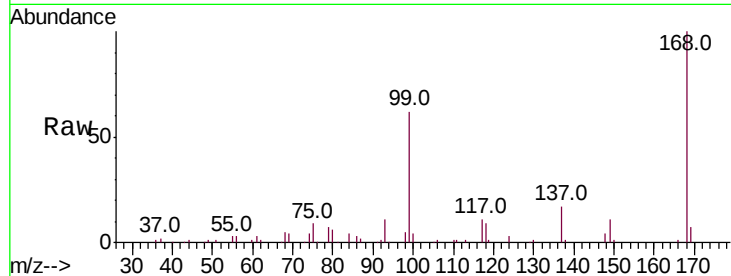


Abundance Ion 167.90 (167.60 to 168.60): VU027314.D (-1169) (-)

Ion 98.90 (98.60 to 99.60): VU027314.D (-1169) (-)

4.99

Time-->

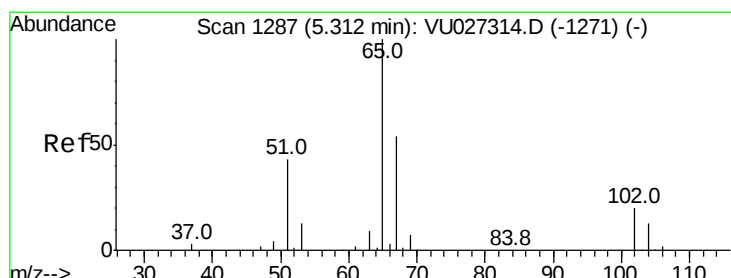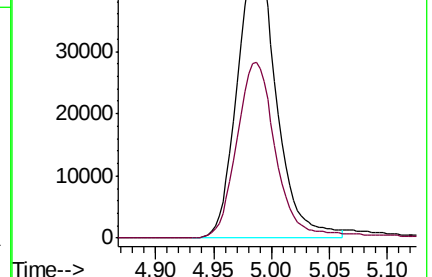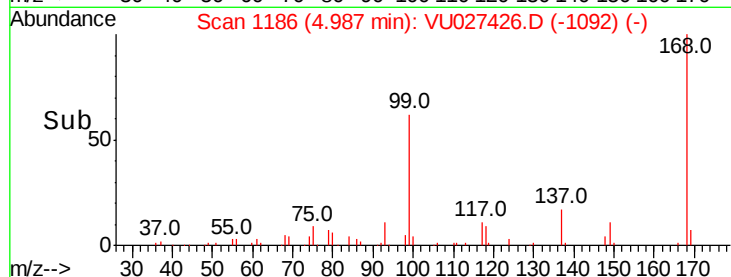

#33

1,2-Dichloroethane-d4

Concen: 58.231 ug/l

RT: 5.31 min Scan# 1287

Delta R.T. 0.00 min

Lab File: VU027426.D


Acq: 04 Oct 2018 22:20

Tgt Ion: 65 Resp: 103182

Ion Ratio Lower Upper

65 100

67 54.1 0.0 107.8


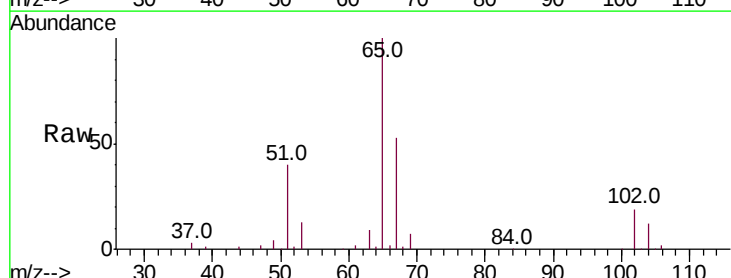



Abundance Ion 64.90 (64.60 to 65.60): VU027314.D (-1271) (-)

Ion 66.90 (66.60 to 67.60): VU027314.D (-1271) (-)

5.31

Time-->

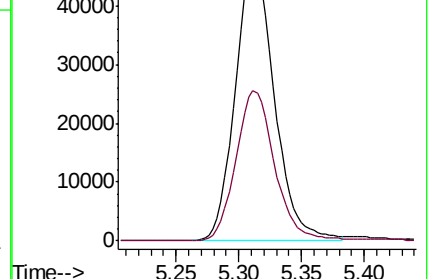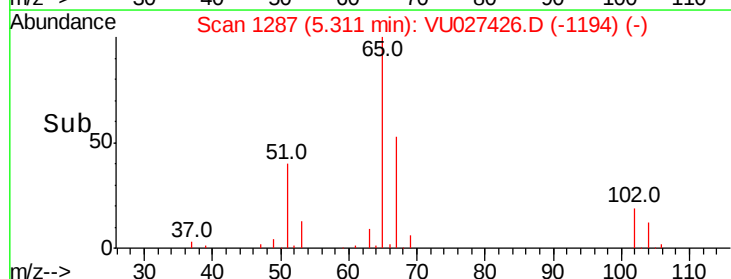


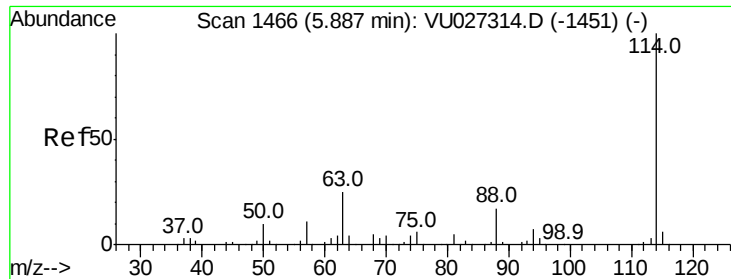




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.89 min Scan# 1467
 Delta R.T. 0.00 min
 Lab File: VU027426.D
 Acq: 04 Oct 2018 22:20

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-8

Tot Ion:114 Resp: 185604
 Ion Ratio Lower Upper
 114 100
 63 24.2 0.0 50.2
 88 17.1 0.0 33.8

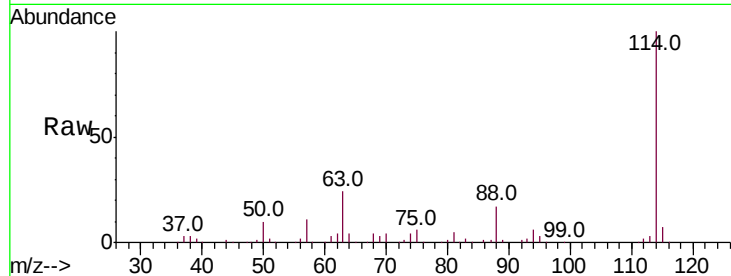


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VU0
 Ion 87.90 (87.60 to 88.60): VU0

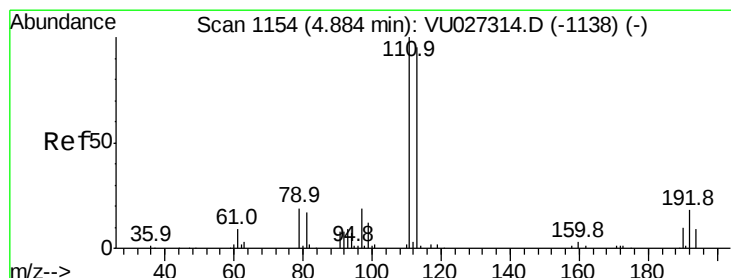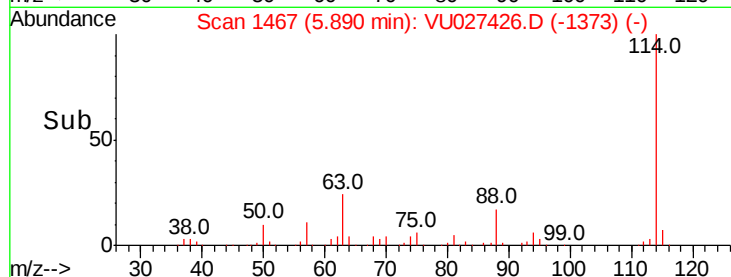
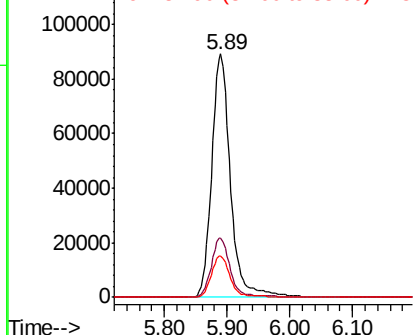



#35
 Dibromofluoromethane
 Concen: 58.284 ug/l
 RT: 4.89 min Scan# 1155
 Delta R.T. 0.00 min
 Lab File: VU027426.D
 Acq: 04 Oct 2018 22:20

Tgt Ion:113 Resp: 74137
 Ion Ratio Lower Upper
 113 100
 111 101.4 83.1 124.7
 192 19.1 15.4 23.0

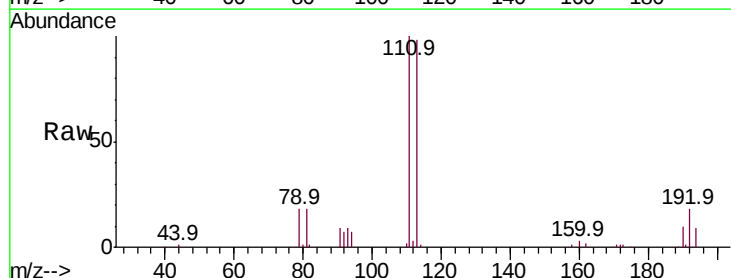

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

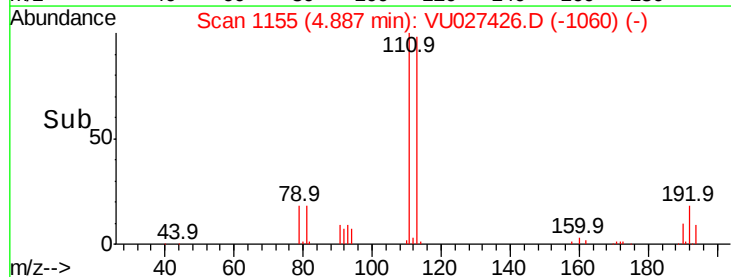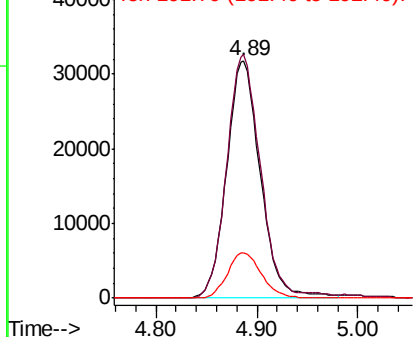

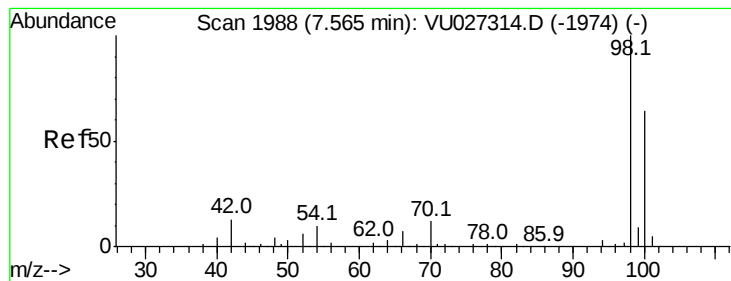

#50

Toluene-d8

Concen: 60.069 ug/l

RT: 7.57 min Scan# 1989

Delta R.T. 0.00 min

Lab File: VU027426.D

Acq: 04 Oct 2018 22:20

Instrument :

MSVOA_U

ClientSampled :


MW-8

Tot Ion: 98 Resp: 285970

Ion Ratio Lower Upper

98 100

100 63.9 52.1 78.1

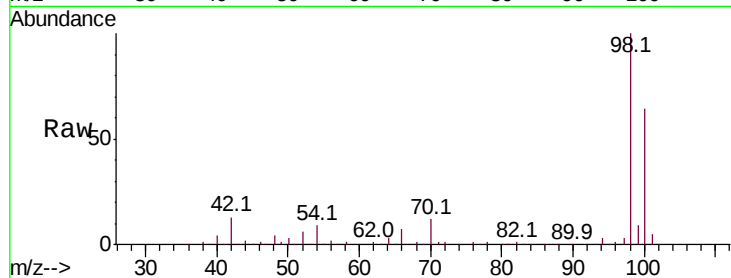

Abundance Ion 98.00 (97.70 to 98.70): VU027314.D (-1974) (-)

Ion 100.00 (99.70 to 100.70): VU027314.D (-1974) (-)

7.57

150000



100000

50000

0

7.50 7.60 7.70

Time-->

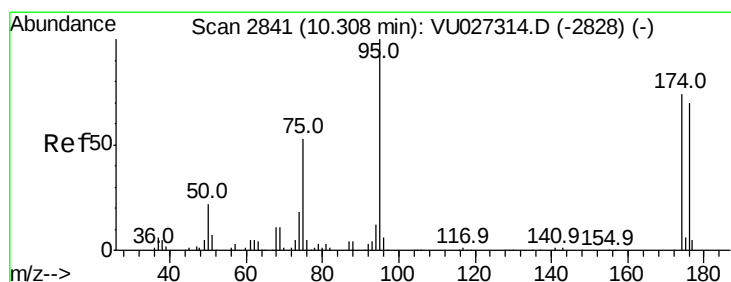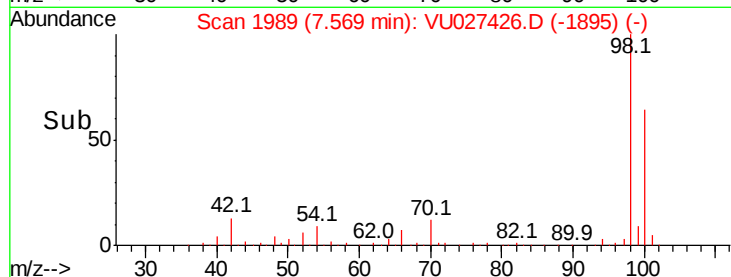

#62

4-Bromofluorobenzene

Concen: 58.215 ug/l

RT: 10.31 min Scan# 2841

Delta R.T. 0.00 min

Lab File: VU027426.D

Acq: 04 Oct 2018 22:20


Tgt Ion: 95 Resp: 102998

Ion Ratio Lower Upper

95 100

174 75.1 0.0 147.8

176 70.1 0.0 140.8

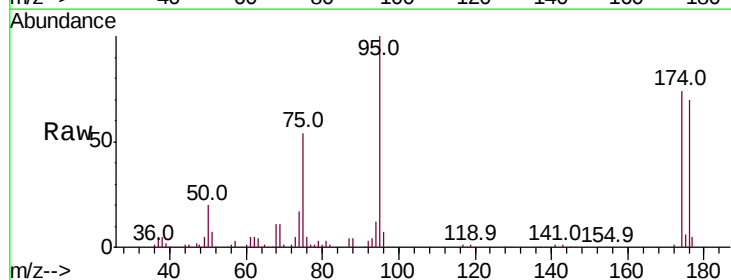

Abundance Ion 94.90 (94.60 to 95.60): VU027314.D (-2828) (-)

Ion 173.80 (173.50 to 174.50): VU027314.D (-2828) (-)

Ion 175.80 (175.50 to 176.50): VU027314.D (-2828) (-)

10.31

80000

60000


40000


20000

0

10.30 10.40

Time-->

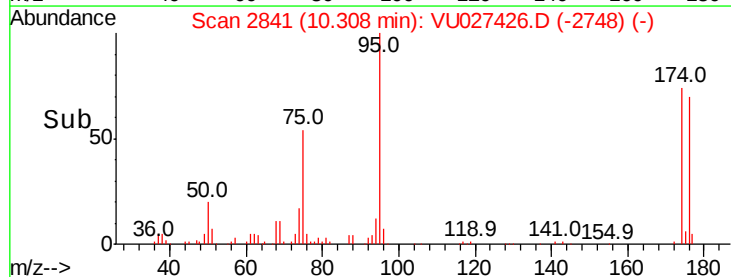


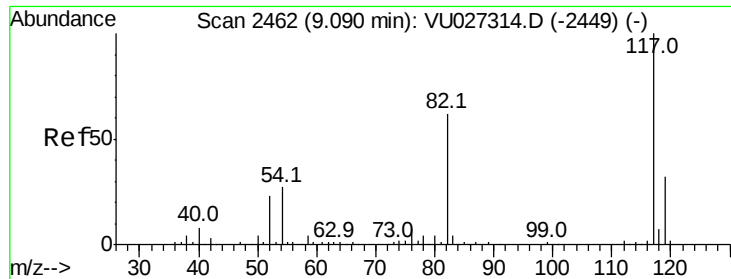




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2463
Delta R.T. 0.00 min
Lab File: VU027426.D
Acq: 04 Oct 2018 22:20

Instrument :
MSVOA_U
ClientSampleId :
MW-8

Tot Ion:117 Resp: 178782
Ion Ratio Lower Upper
117 100
82 60.8 49.2 73.8
119 32.3 25.7 38.5

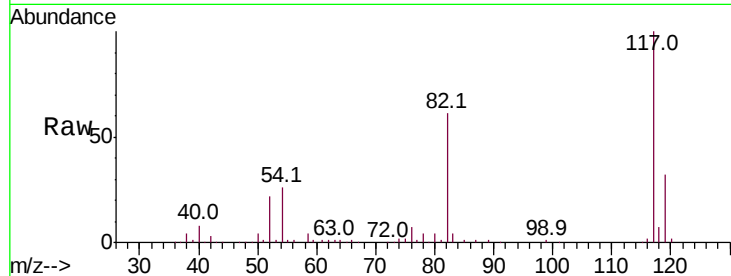


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

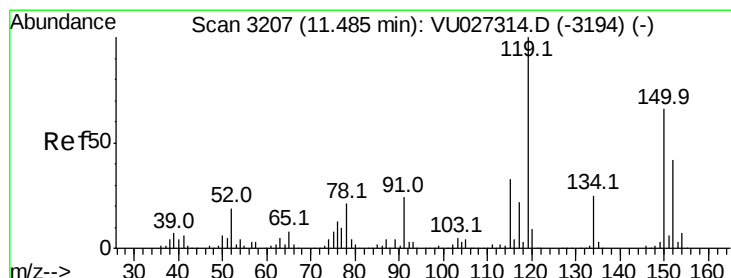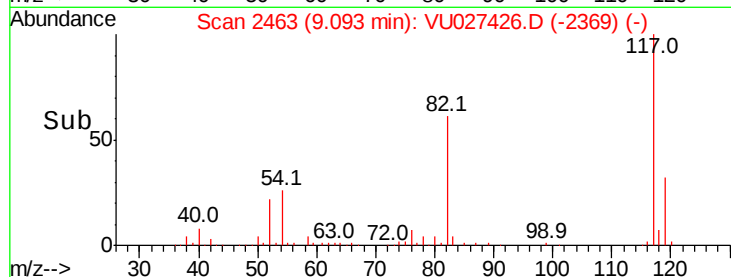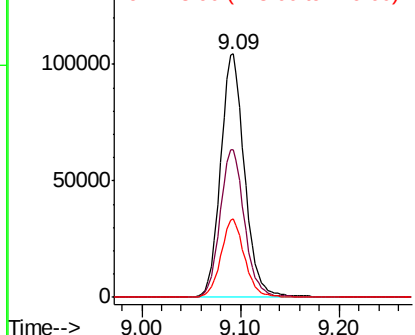

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3207
Delta R.T. -0.00 min
Lab File: VU027426.D
Acq: 04 Oct 2018 22:20

Tgt Ion:152 Resp: 95300
Ion Ratio Lower Upper
152 100
115 60.9 43.4 130.2
150 158.7 0.0 349.2

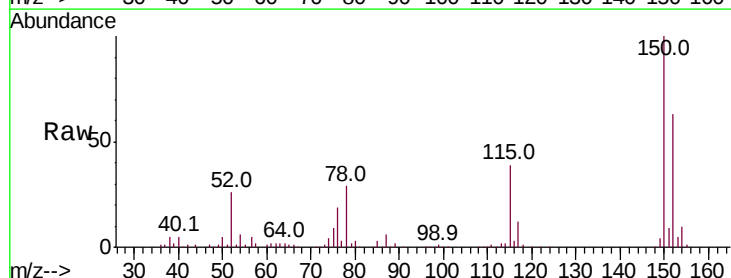

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

