


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100418\
Data File : VU027411.D
Acq On : 04 Oct 2018 16:14
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Title : SW846 8260
Last Update : Tue Oct 02 02:04:34 2018

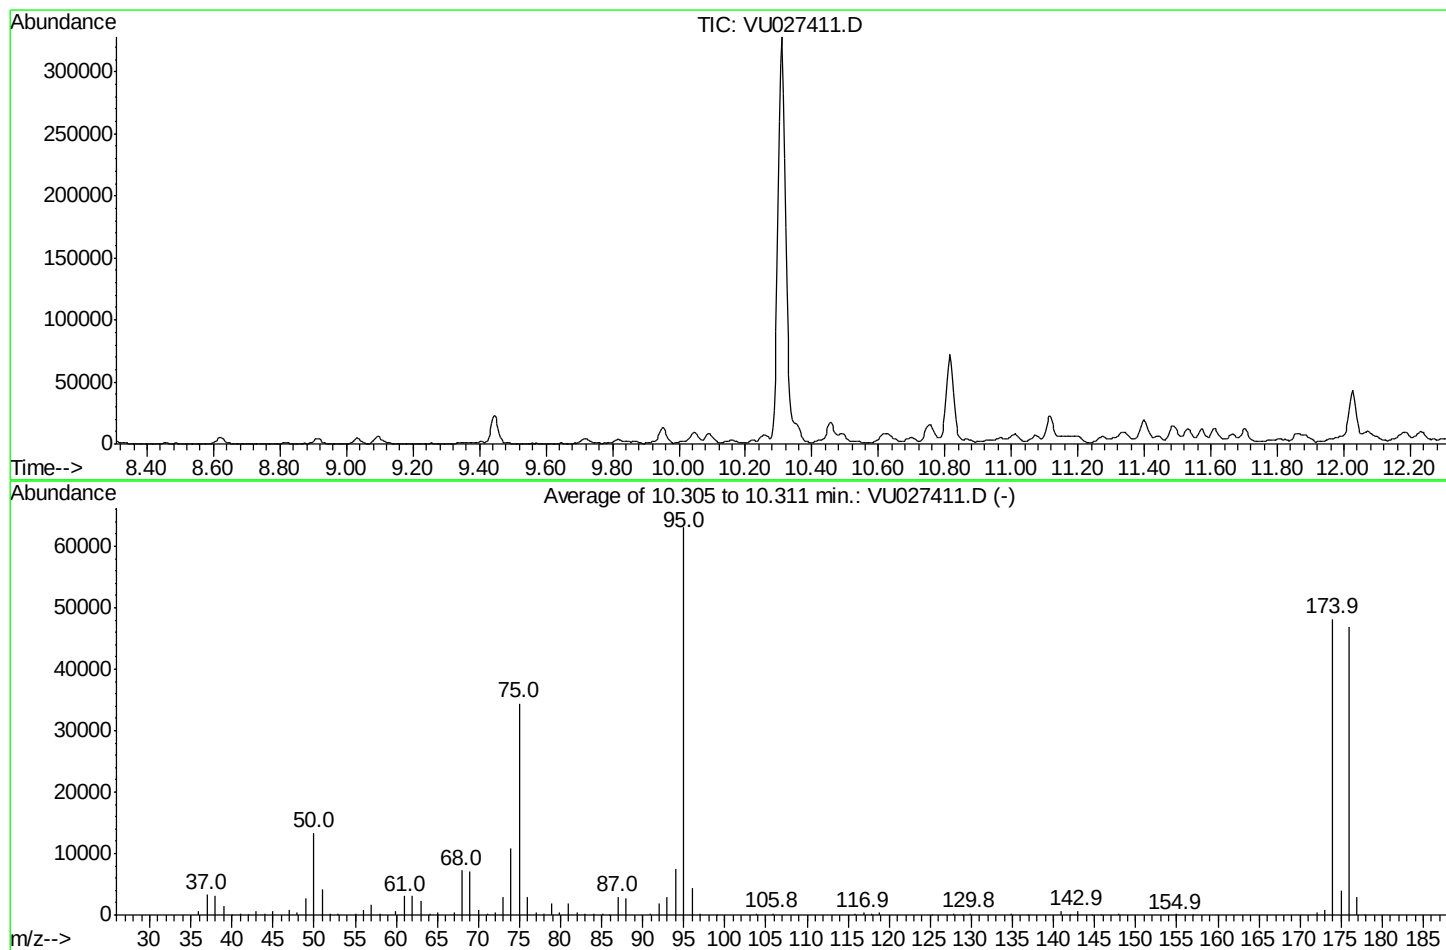

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	13411	PASS
75	95	30	60	54.5	34376	PASS
95	95	100	100	100.0	63080	PASS
96	95	5	9	7.0	4385	PASS
173	174	0.00	2	1.5	741	PASS
174	95	50	100	76.4	48168	PASS
175	174	5	9	8.3	4006	PASS
176	174	95	101	97.2	46813	PASS
177	176	5	9	6.2	2898	PASS