

Data File : VU034931.D
Acq On : 04 Oct 2019 13:10
Operator : JC/SP
Sample : K5201-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB7

Quant Time: Oct 14 08:10:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR093019WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 05 00:29:19 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	203778	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	200474	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.46	152	91283	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	72833	5.05	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.00%
7) Chloroethane-d5	1.68	69	61813	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.00%
11) 1,1-Dichloroethene-d2	2.26	63	100176	4.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.00%
20) 2-Butanone-d5	4.17	46	177669	43.26	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.52%
24) Chloroform-d	4.62	84	123541	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
26) 1,2-Dichloroethane-d4	5.29	65	70145	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
32) Benzene-d6	5.32	84	256729	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.80%
36) 1,2-Dichloropropane-d6	6.31	67	84251	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.00%
41) Toluene-d8	7.54	98	234576	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
43) trans-1,3-Dichloropropene-	7.83	79	28789	4.74	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.80%
46) 2-Hexanone-d5	8.30	63	144158	48.09	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.18%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	67706	5.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.80%
64) 1,2-Dichlorobenzene-d4	11.84	152	85950	5.68	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.60%


Target Compounds					Qvalue
3) Chloromethane	1.32	50	2415	0.245 ug/L	93
13) Acetone	2.31	43	7646	2.544 ug/L	99
42) Toluene	7.62	91	4694	0.107 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU034931.D
Acq On : 04 Oct 2019 13:10
Operator : JC/SP
Sample : K5201-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB7

Quant Time: Oct 14 08:10:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR093019WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 05 00:29:19 2019
Response via : Initial Calibration

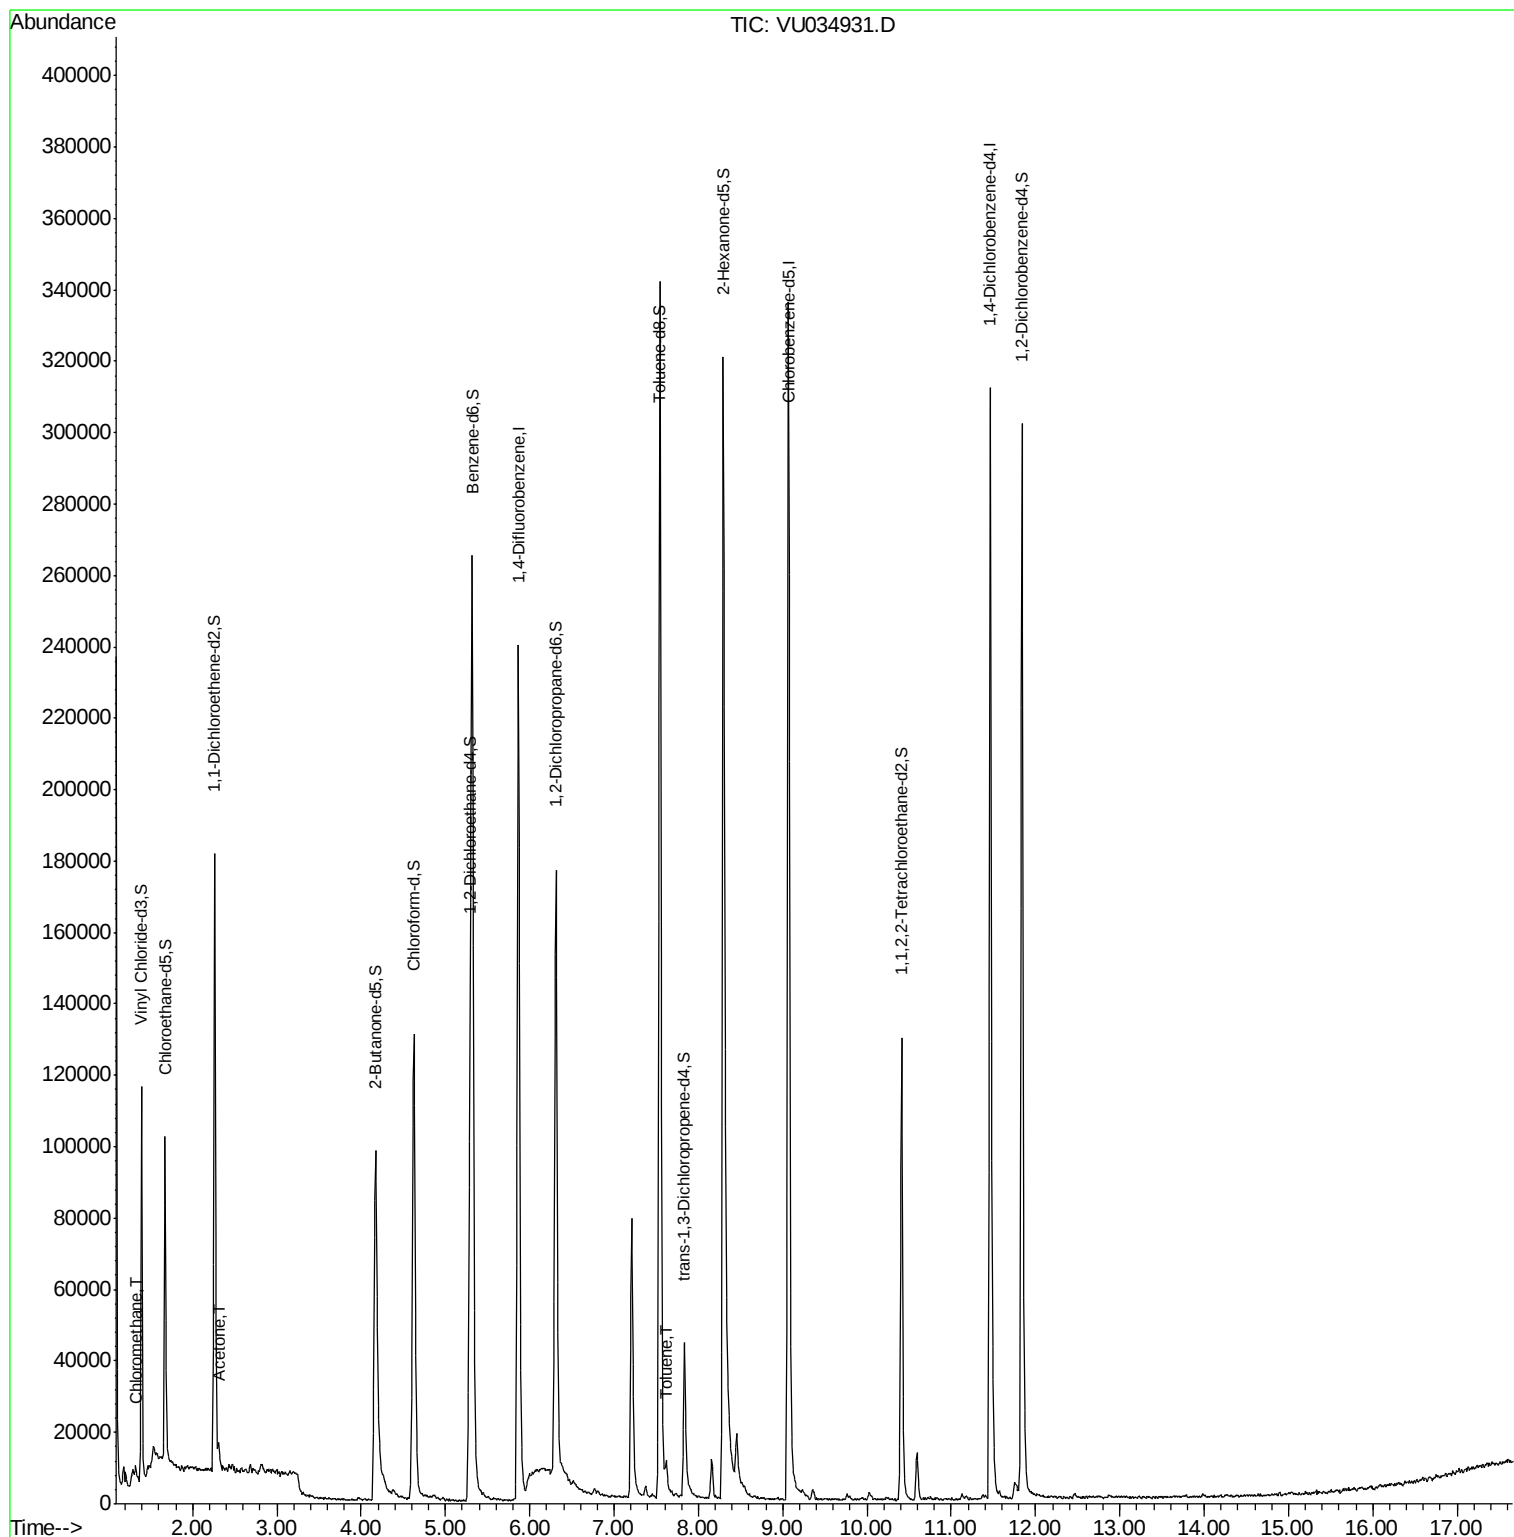

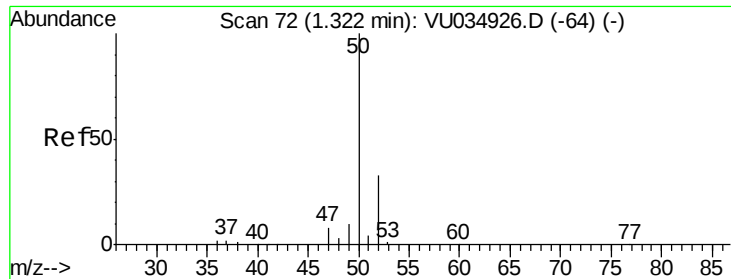

#3

Chloromethane

Concen: 0.245 ug/L

RT: 1.32 min Scan# 73

Delta R.T. 0.00 min

Lab File: VU034931.D

Acq: 04 Oct 2019 13:10

Instrument :

MSVOA_U

ClientSampleId :


C0AB7

Tgt Ion: 50 Resp: 2415

Ion Ratio Lower Upper




50 100

52 36.3 22.7 42.1

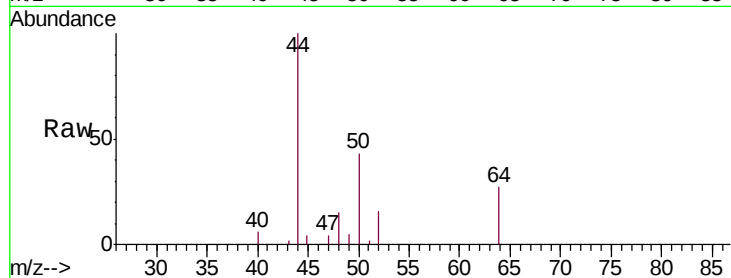

Abundance Ion 50.05 (49.75 to 50.75): VU034926.D (-64) (-)

Ion 52.05 (51.75 to 52.75): VU034926.D (-64) (-)

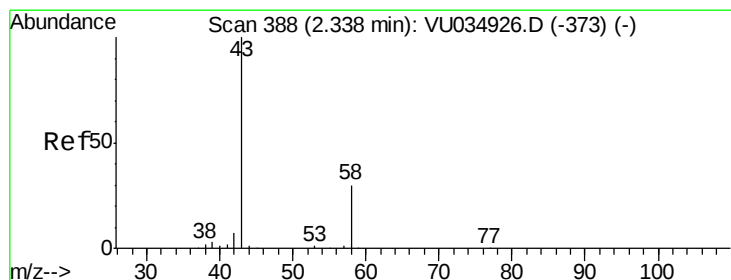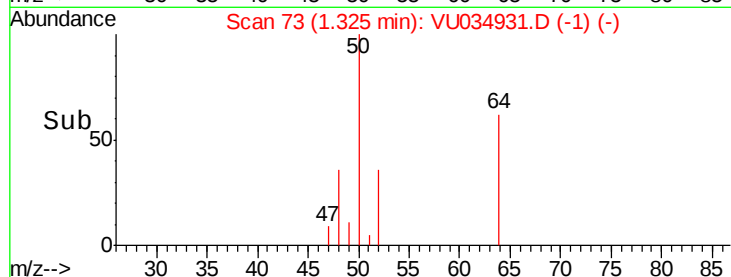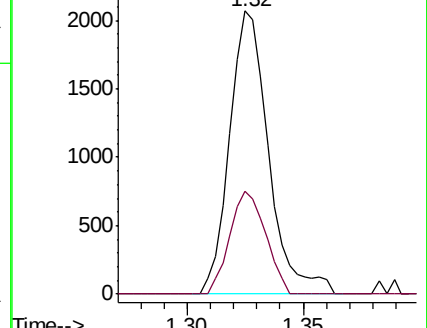

#13

Acetone

Concen: 2.544 ug/L

RT: 2.31 min Scan# 379

Delta R.T. -0.03 min

Lab File: VU034931.D


Acq: 04 Oct 2019 13:10

Tgt Ion: 43 Resp: 7646

Ion Ratio Lower Upper



43 100


58 26.4 0.0 54.0

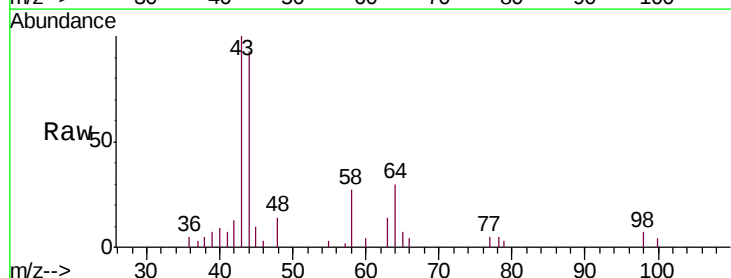

Abundance Ion 43.05 (42.75 to 43.75): VU034926.D (-373) (-)

Ion 58.05 (57.75 to 58.75): VU034926.D (-373) (-)

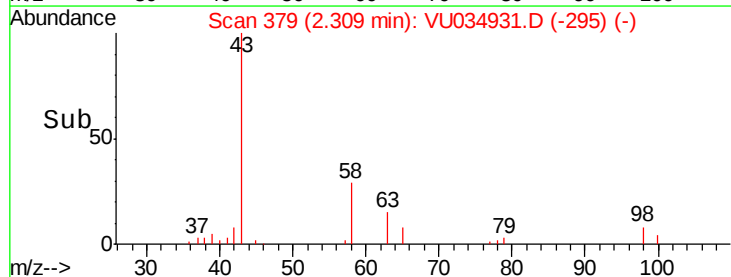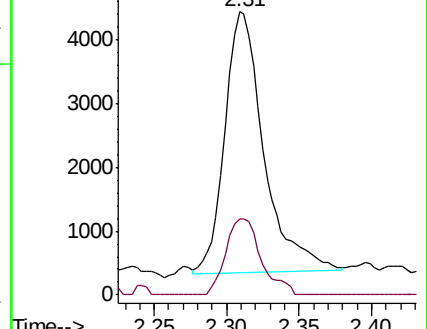

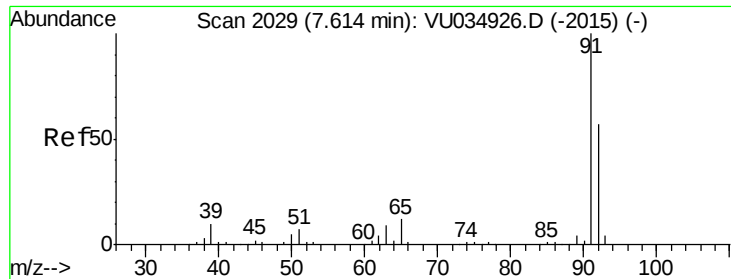

#42

Toluene

Concen: 0.107 ug/L

RT: 7.62 min Scan# 2031

Delta R.T. 0.01 min

Lab File: VU034931.D

Acq: 04 Oct 2019 13:10

Instrument :

MSVOA_U

ClientSampleId :

C0AB7

Tgt Ion: 91 Resp: 4694

Ion Ratio Lower Upper

91 100

92 64.2 39.3 72.9

