

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U100419\
 Data File : VU034940.D
 Acq On : 04 Oct 2019 17:14
 Operator : JC/SP
 Sample : K5201-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AB9

Quant Time: Oct 05 04:07:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR093019WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 05 00:29:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	194182	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	194132	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.46	152	79957	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	69943	5.09	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.80%
7) Chloroethane-d5	1.68	69	58805	5.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.80%
11) 1,1-Dichloroethene-d2	2.26	63	94299	4.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.00%
20) 2-Butanone-d5	4.17	46	167530	42.81	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.62%
24) Chloroform-d	4.62	84	119026	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
26) 1,2-Dichloroethane-d4	5.29	65	65801	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
32) Benzene-d6	5.32	84	244410	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.20%
36) 1,2-Dichloropropane-d6	6.31	67	82261	5.15	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.00%
41) Toluene-d8	7.54	98	223198	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
43) trans-1,3-Dichloropropene-	7.84	79	24547	4.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.40%
46) 2-Hexanone-d5	8.30	63	129004	44.44	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.88%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	62944	4.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.80%
64) 1,2-Dichlorobenzene-d4	11.84	152	77751	5.86	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.20%


Target Compounds					Ovalue
13) Acetone	2.31	43	4811	1.680 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100419\
Data File : VU034940.D
Acq On : 04 Oct 2019 17:14
Operator : JC/SP
Sample : K5201-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB9

Quant Time: Oct 05 04:07:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR093019WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 05 00:29:19 2019
Response via : Initial Calibration

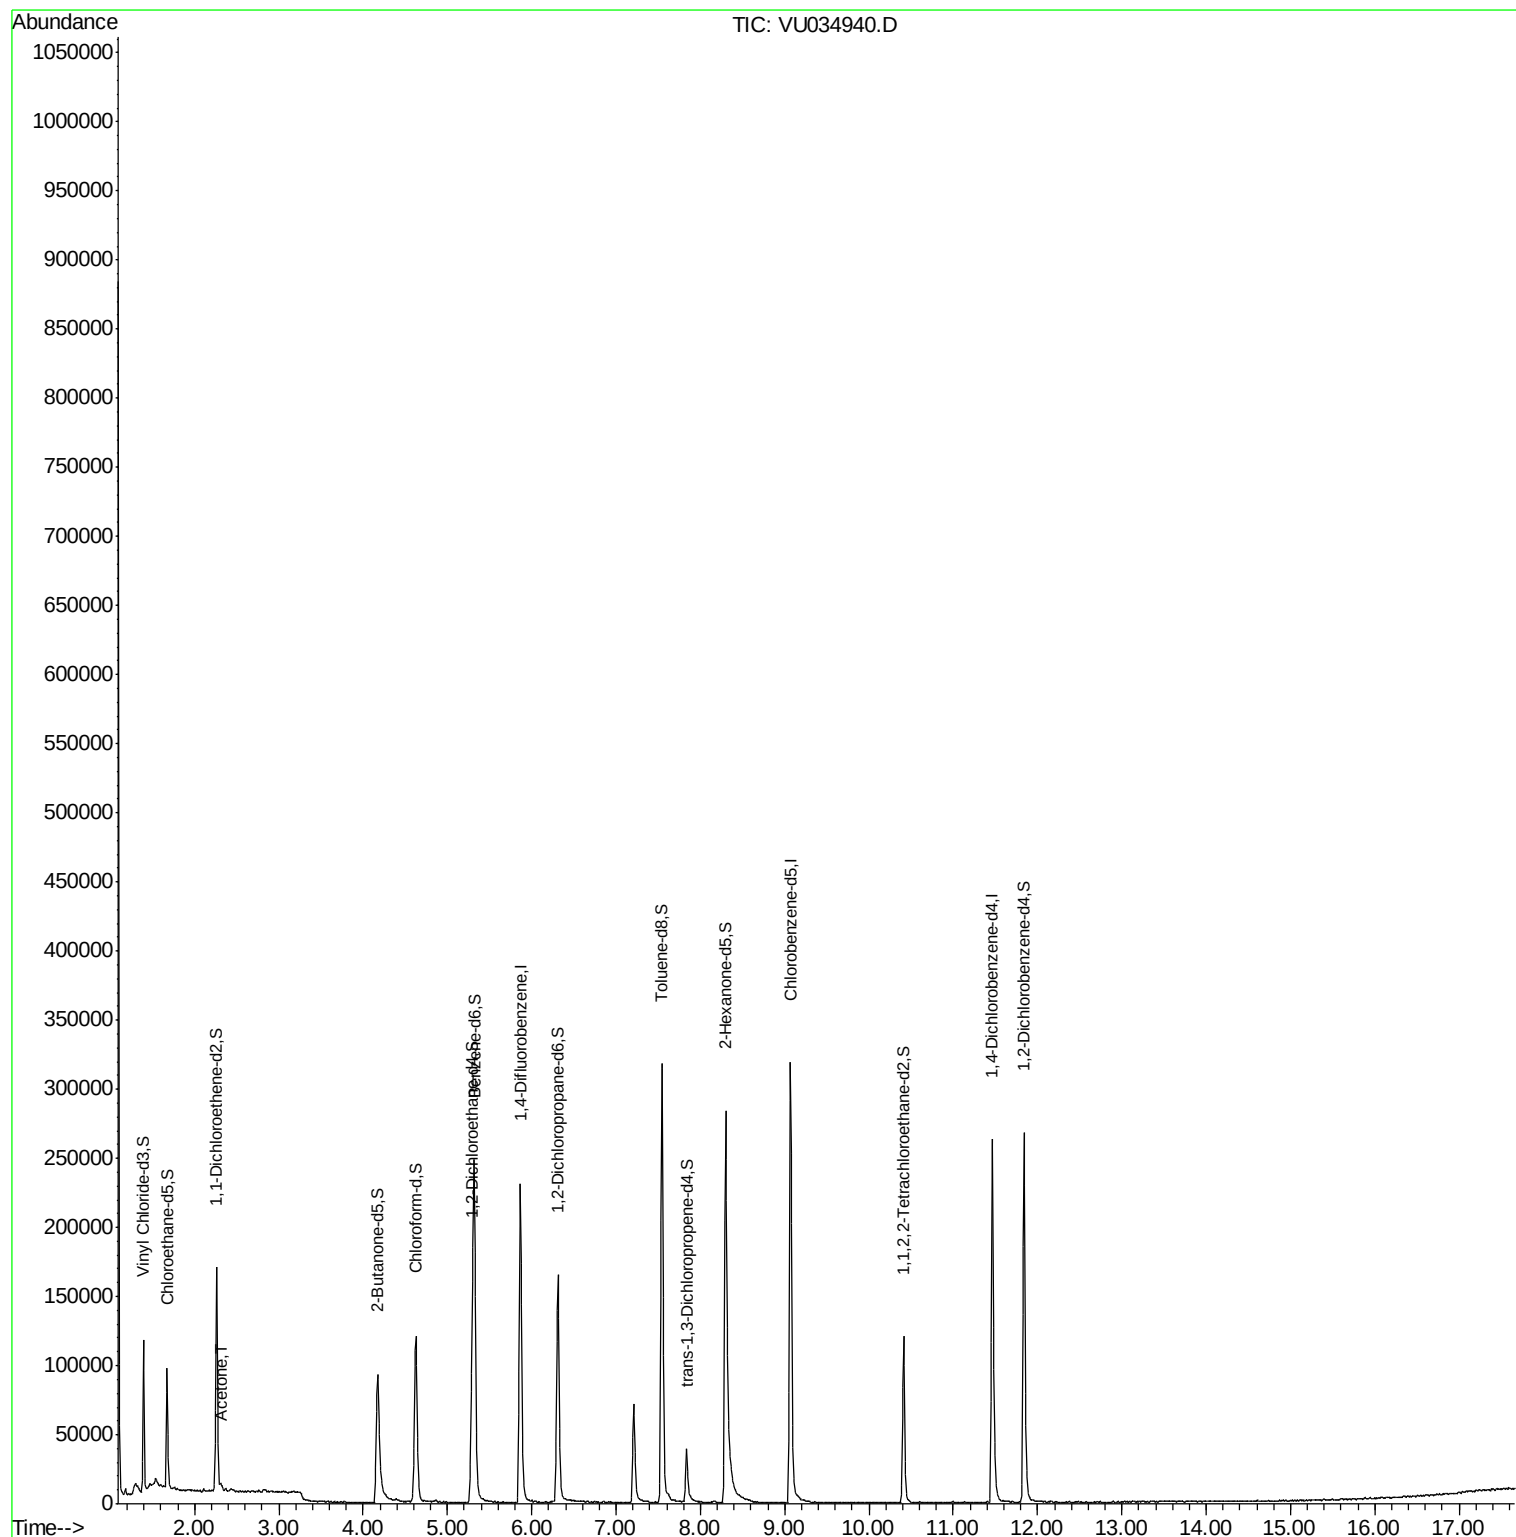

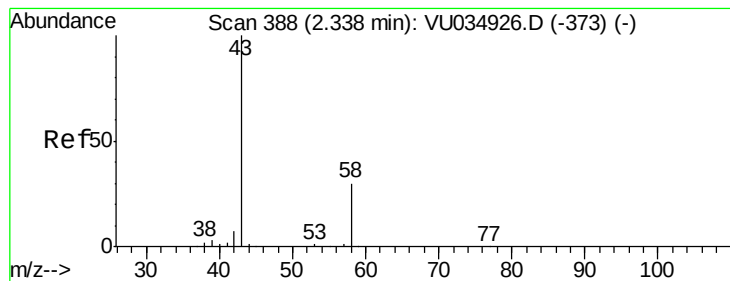

#13
 Acetone
 Concen: 1.680 ug/L
 RT: 2.31 min Scan# 379
 Delta R.T. -0.03 min
 Lab File: VU034940.D
 Acq: 04 Oct 2019 17:14

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AB9

Tot Ion: 43 Resp: 4811
 Ion Ratio Lower Upper
 43 100
 58 32.2 0.0 54.0

