

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100419\
 Data File : VU034942.D
 Acq On : 04 Oct 2019 18:02
 Operator : JC/SP
 Sample : K5201-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AC1

Quant Time: Oct 05 04:15:27 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR093019WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 05 00:29:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	193973	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	189669	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.46	152	84244	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	71803	5.23	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.60%
7) Chloroethane-d5	1.67	69	61305	5.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.40%
11) 1,1-Dichloroethene-d2	2.26	63	98270	4.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.40%
20) 2-Butanone-d5	4.17	46	176308	45.10	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.20%
24) Chloroform-d	4.62	84	121863	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.00%
26) 1,2-Dichloroethane-d4	5.29	65	69151	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.32	84	250285	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.00%
36) 1,2-Dichloropropane-d6	6.31	67	84659	5.42	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.40%
41) Toluene-d8	7.54	98	233464	5.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.00%
43) trans-1,3-Dichloropropene-	7.83	79	26879	4.67	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.40%
46) 2-Hexanone-d5	8.30	63	136966	48.30	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.60%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	63980	5.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.80%
64) 1,2-Dichlorobenzene-d4	11.84	152	82540	5.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.20%


Target Compounds					Ovalue
13) Acetone	2.31	43	4299	1.502 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100419\
Data File : VU034942.D
Acq On : 04 Oct 2019 18:02
Operator : JC/SP
Sample : K5201-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AC1

Quant Time: Oct 05 04:15:27 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR093019WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 05 00:29:19 2019
Response via : Initial Calibration

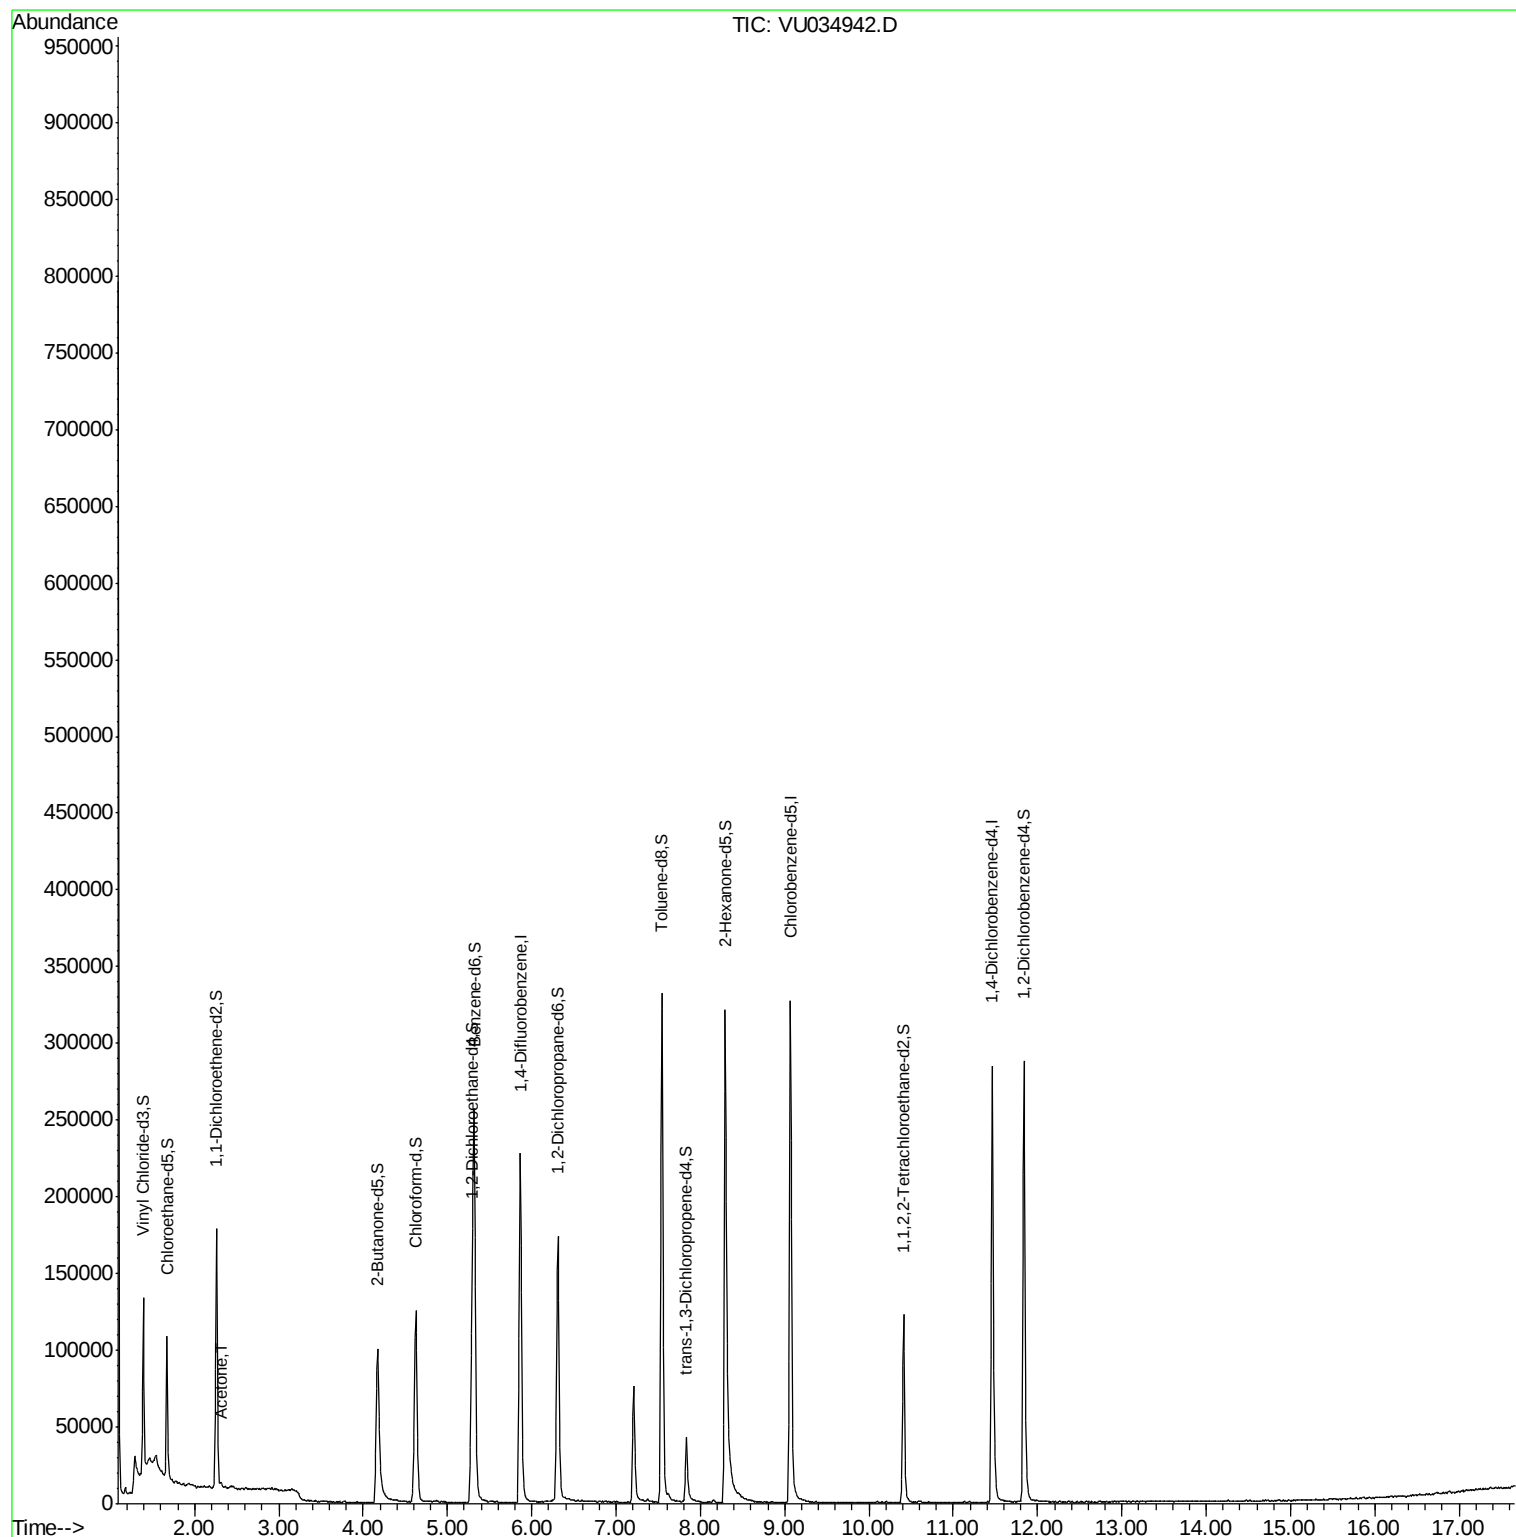

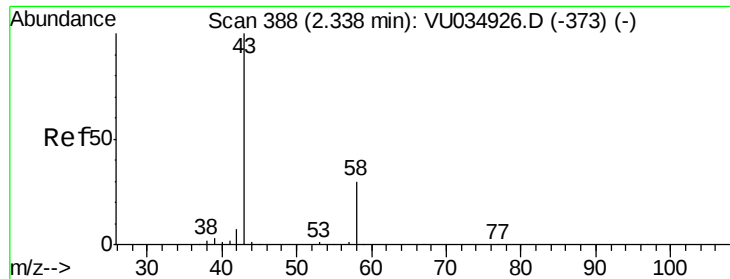

#13

Acetone

Concen: 1.502 ug/L

RT: 2.31 min Scan# 380

Delta R.T. -0.03 min

Lab File: VU034942.D

Acq: 04 Oct 2019 18:02

Instrument :

MSVOA_U

ClientSampleId :

C0AC1

Tot Ion: 43 Resp: 4299

Ion Ratio Lower Upper

43 100

58 30.9 0.0 54.0

