


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100419\
 Data File : VU034925.D
 Acq On : 04 Oct 2019 09:54
 Operator : JC/SP
 Sample : BFB13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB13

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR093019WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Oct 05 00:29:19 2019

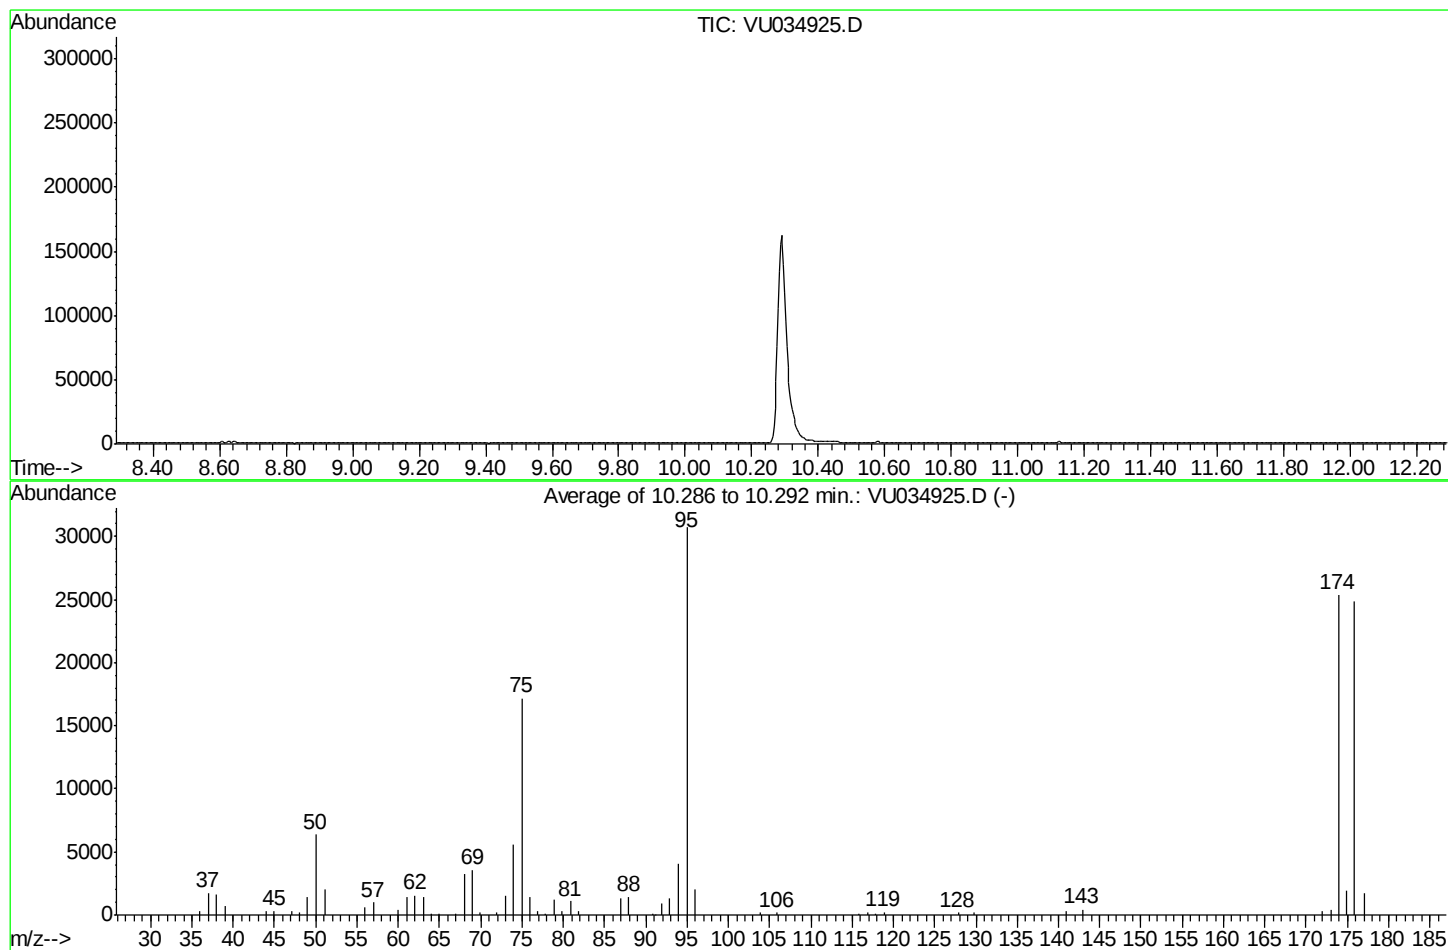

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	6365	PASS
75	95	30	80	55.9	17173	PASS
95	95	100	100	100.0	30722	PASS
96	95	5	9	6.7	2063	PASS
173	174	0.00	2	1.6	412	PASS
174	95	50	120	82.7	25408	PASS
175	174	5	9	7.5	1908	PASS
176	174	95	101	97.8	24861	PASS
177	176	5	9	6.9	1705	PASS

m/z	Abundance
35.00	262.0
37.00	1710.0
38.00	1646.0
39.00	778.0
39.80	191.0
44.00	811.0
45.00	317.0
47.00	339.0
48.00	243.0
49.00	1416.0
50.00	6434.0
51.00	2161.0
56.00	566.0
57.00	887.0
59.90	398.0
61.00	1386.0
62.00	1498.0
63.00	1409.0
64.00	127.0
64.90	111.0
68.00	3190.0
69.00	3577.0
69.90	237.0
71.90	149.0
73.00	1581.0
74.00	5414.0
75.00	16920.0
76.00	1569.0
76.90	228.0
77.80	144.0
78.90	1314.0
79.80	323.0
80.90	1120.0
81.80	293.0
87.00	1216.0
88.00	1340.0
90.90	124.0
91.90	856.0
92.90	1277.0
94.00	4106.0
95.00	29944.0
96.00	2173.0
103.80	200.0
105.90	187.0
115.80	119.0
116.90	201.0
117.80	143.0
118.90	191.0
127.80	188.0
129.80	178.0
140.90	329.0
143.00	397.0
171.90	206.0
172.90	390.0
173.90	24816.0
174.90	1772.0
175.90	24232.0
177.00	1731.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
35.90	287.0
37.00	1771.0
38.00	1625.0
39.00	749.0
39.80	226.0
44.00	909.0
45.00	319.0
47.10	312.0
48.00	217.0
49.00	1489.0
50.00	6568.0
51.00	2105.0
56.00	625.0
57.00	1047.0
59.90	426.0
61.00	1490.0
62.00	1616.0
63.00	1422.0
63.90	134.0
64.90	110.0
66.90	106.0
68.00	3386.0
69.00	3702.0
69.90	269.0
72.00	201.0
73.00	1524.0
74.00	5764.0
75.00	17632.0
76.00	1519.0
77.00	267.0
77.70	136.0
78.90	1268.0
79.80	341.0
80.90	1101.0
81.80	338.0
87.00	1375.0
87.90	1570.0
90.80	115.0
91.90	989.0
92.90	1280.0
94.00	4320.0
95.00	31544.0
96.00	2098.0
103.80	186.0
105.90	192.0
115.80	135.0
116.90	183.0
117.80	154.0
118.90	215.0
127.90	211.0
129.80	195.0
140.90	382.0
142.90	415.0
172.00	286.0
173.00	436.0
173.90	26096.0
174.90	1938.0
175.90	25728.0
177.00	1777.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
35.90	273.0
37.00	1723.0
38.00	1504.0
39.00	751.0
39.90	260.0
44.00	929.0
45.00	298.0
47.10	309.0
48.10	215.0
49.00	1375.0
50.00	6095.0
51.10	1882.0
56.00	583.0
57.00	1099.0
59.90	376.0
61.00	1455.0
62.00	1547.0
63.00	1410.0
63.90	158.0
64.90	148.0
66.90	113.0
68.00	3206.0
69.00	3377.0
70.00	247.0
72.00	189.0
73.00	1448.0
74.00	5607.0
75.00	16968.0
76.00	1292.0
77.00	283.0
77.70	115.0
78.90	1149.0
79.80	319.0
80.90	1045.0
81.80	365.0
87.00	1380.0
87.90	1495.0
91.10	126.0
91.90	973.0
92.90	1270.0
94.00	3889.0
95.00	30680.0
96.00	1918.0
103.90	155.0
105.90	178.0
115.80	128.0
116.90	169.0
117.80	152.0
118.90	215.0
127.90	194.0
129.80	187.0
140.90	348.0
142.90	436.0
172.00	299.0
173.10	410.0
173.90	25312.0
174.90	2014.0
175.90	24624.0
177.00	1607.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

Scan 2848 (10.247 min): VU034925.D
BFB13

m/z	Abundance
39.90	242.0
43.90	576.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13